
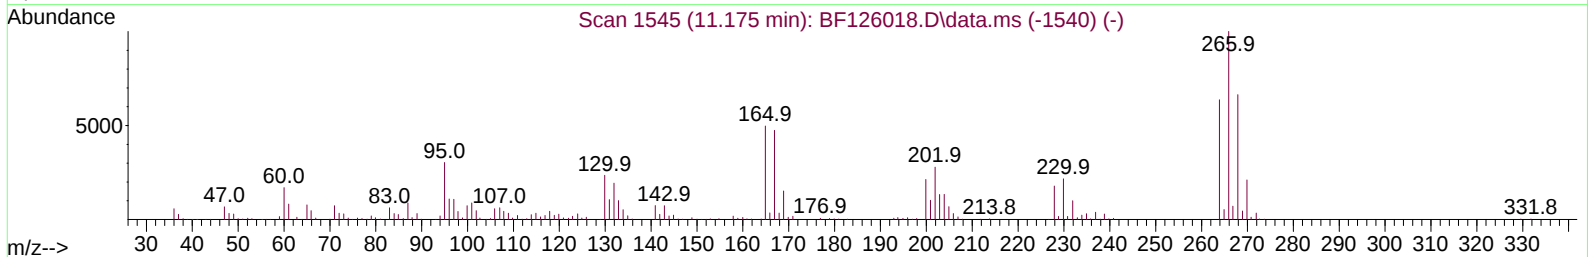
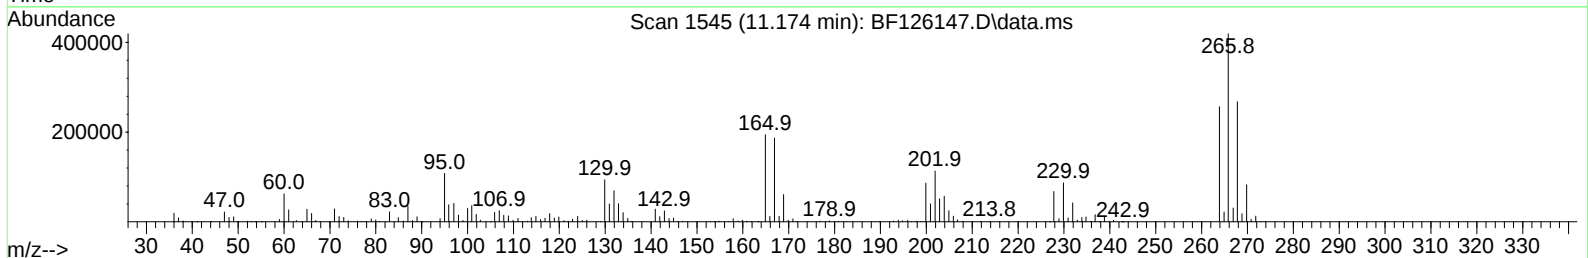


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
 Data File : BF126147.D
 Acq On : 12 Nov 2021 9:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:37:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 08:09:33 2021
 Response via : Initial Calibration

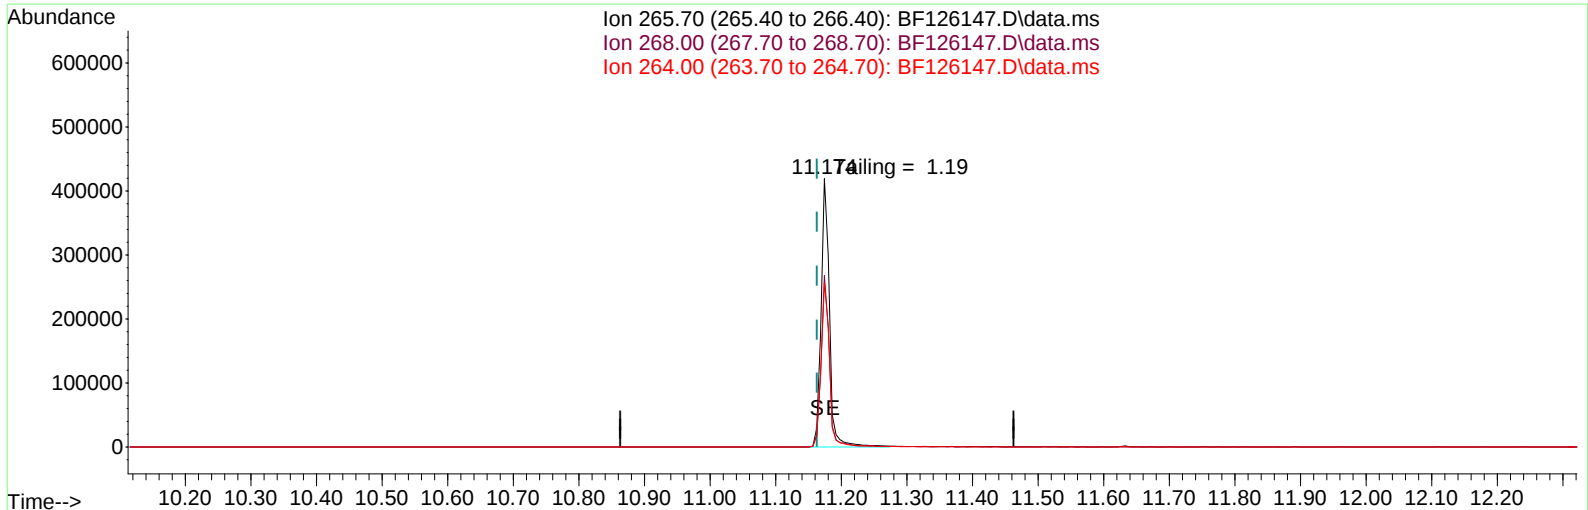

TIC: BF126147.D\data.ms

(70) Pentachlorophenol (C)




11.174min (+ 0.012) 25661.54 ng

response 373543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.84
264.00	69.90	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
 Data File : BF126147.D
 Acq On : 12 Nov 2021 9:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 08:37:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 08:09:33 2021
 Response via : Initial Calibration

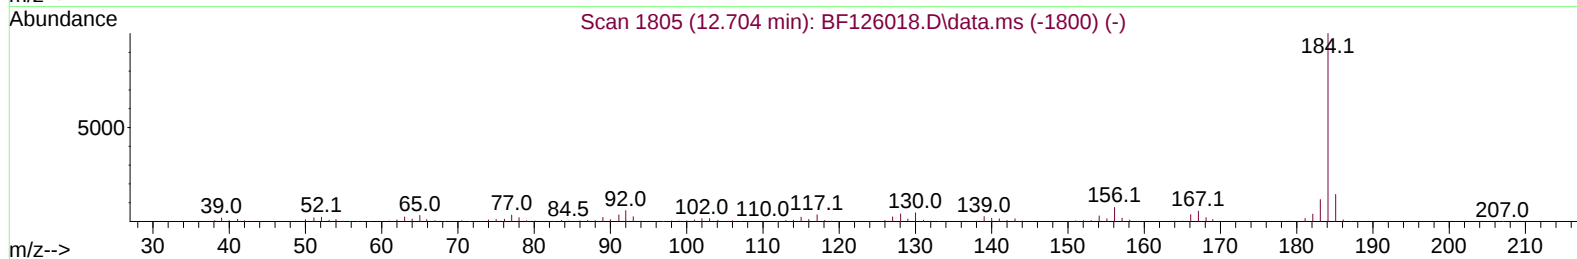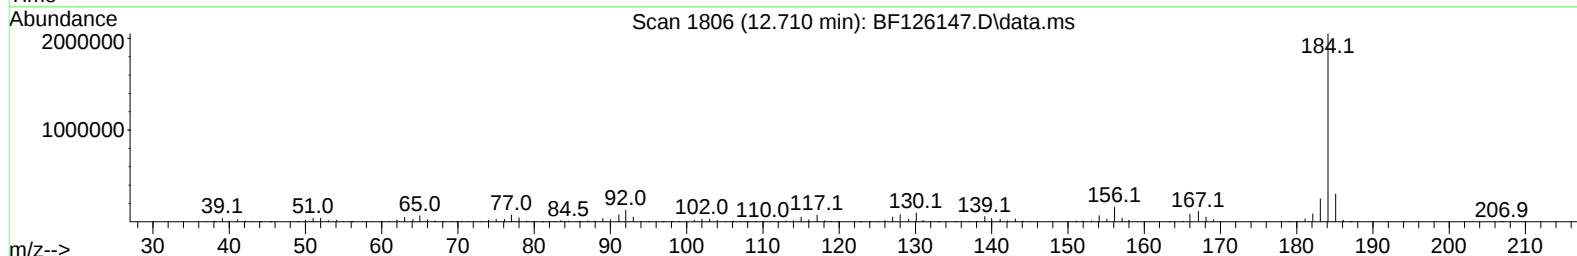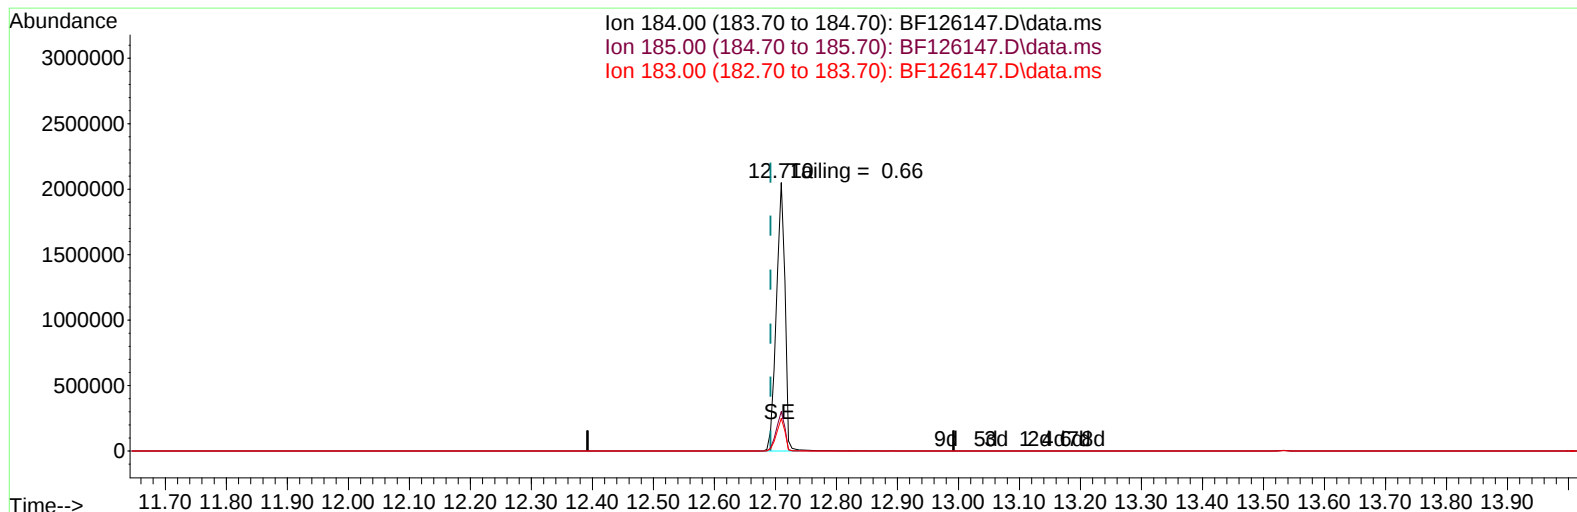

TIC: BF126147.D\data.ms

(77) Benzidine

12.710min (+ 0.017) 470308.37 ng m

response 2012406

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.74
183.00	10.10	12.19#
0.00	0.00	0.00