

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
 Data File : BF126152.D
 Acq On : 12 Nov 2021 12:37
 Operator : JU/CG
 Sample : M4607-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 207

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.540	241	247	256	rVB	50895	82673	1.42%	0.250%
2	4.440	389	400	403	rBV	3103978	3914951	67.11%	11.846%
3	5.063	499	506	509	rBV	2313213	2841523	48.71%	8.598%
4	5.463	569	574	577	rBV	2128934	2049124	35.12%	6.200%
5	6.475	740	746	749	rBV	3050754	3000702	51.44%	9.079%
6	6.845	805	809	812	rBV	903928	781267	13.39%	2.364%
7	7.163	859	863	866	rBV	122039	98734	1.69%	0.299%
8	7.404	899	904	907	rBV	2708420	2327847	39.90%	7.044%
9	8.028	1007	1010	1023	rBV	168867	259814	4.45%	0.786%
10	8.128	1023	1027	1030	rBV	1090231	973637	16.69%	2.946%
11	9.204	1205	1210	1213	rBV	5633506	4614080	79.09%	13.961%
12	9.880	1321	1325	1328	rBV	1509321	1209543	20.73%	3.660%
13	10.663	1455	1458	1466	rBV	1177273	1040089	17.83%	3.147%
14	11.363	1574	1577	1581	rBV	1513764	1329810	22.79%	4.024%
15	11.763	1641	1645	1648	rVB	95097	77009	1.32%	0.233%
16	12.957	1843	1848	1851	rBV	6839849	5833905	100.00%	17.652%
17	13.874	1999	2004	2019	rBV5	159446	357204	6.12%	1.081%
18	14.004	2021	2026	2030	rVV	1327364	1181871	20.26%	3.576%
19	14.768	2152	2156	2158	rBV	120643	124757	2.14%	0.377%
20	14.862	2169	2172	2179	rVB2	82285	92065	1.58%	0.279%
21	15.474	2270	2276	2280	rBV	688953	858789	14.72%	2.599%




Sum of corrected areas: 33049394

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
Data File : BF126152.D
Acq On : 12 Nov 2021 12:37
Operator : JU/CG
Sample : M4607-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
207

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

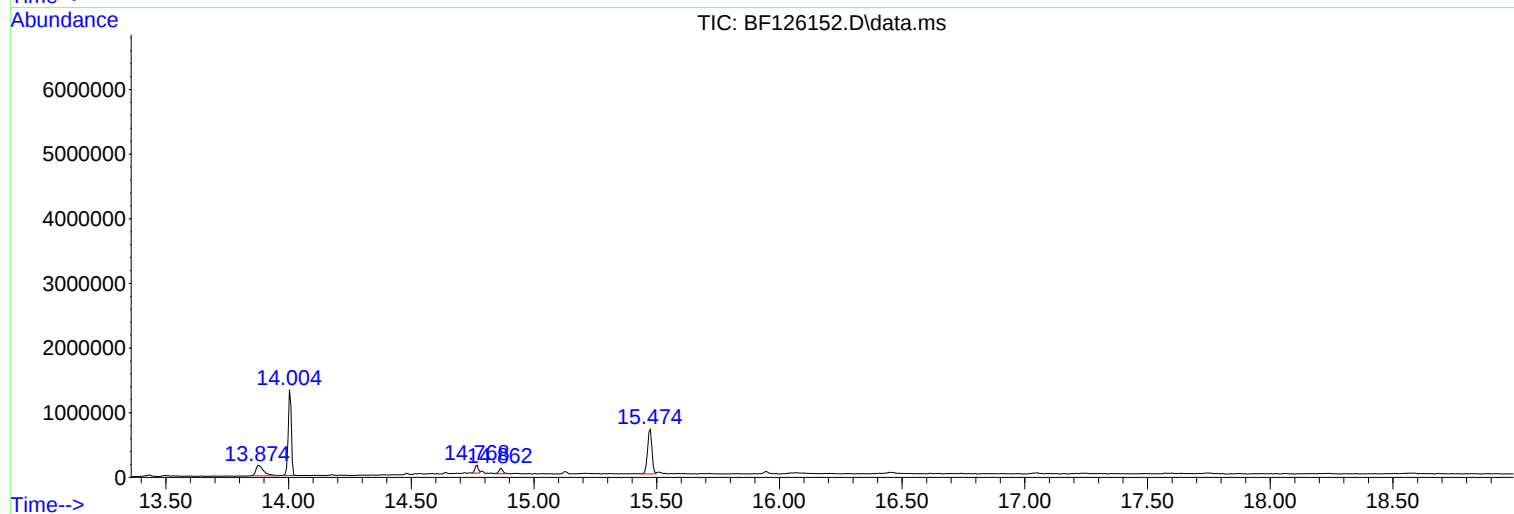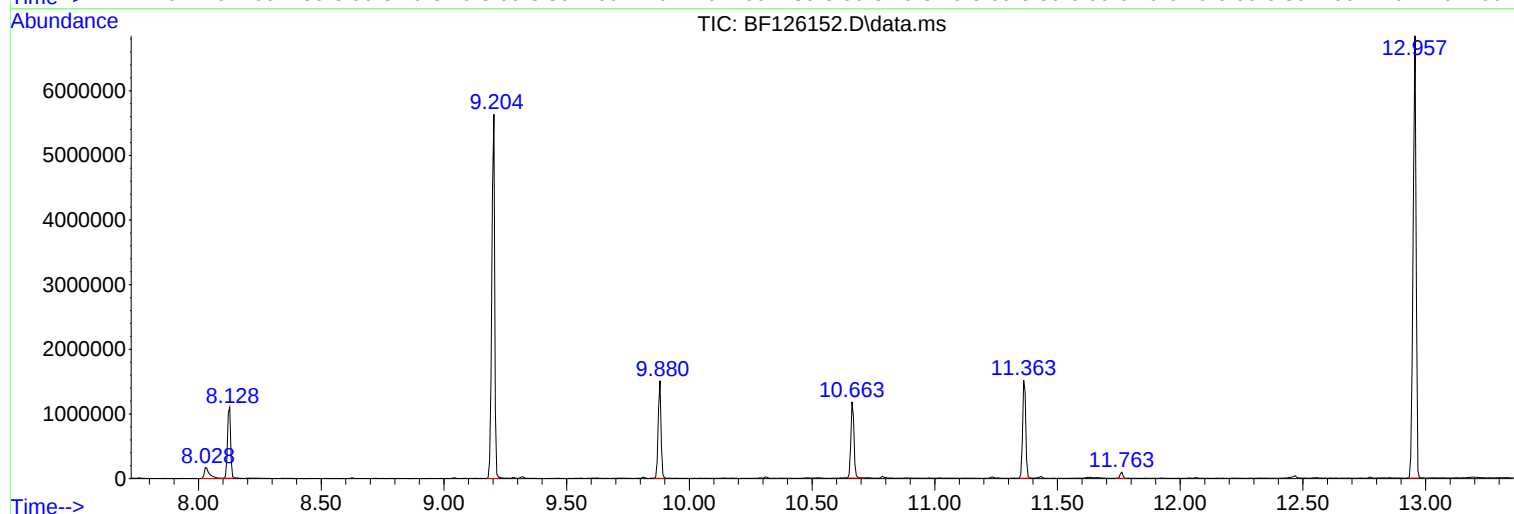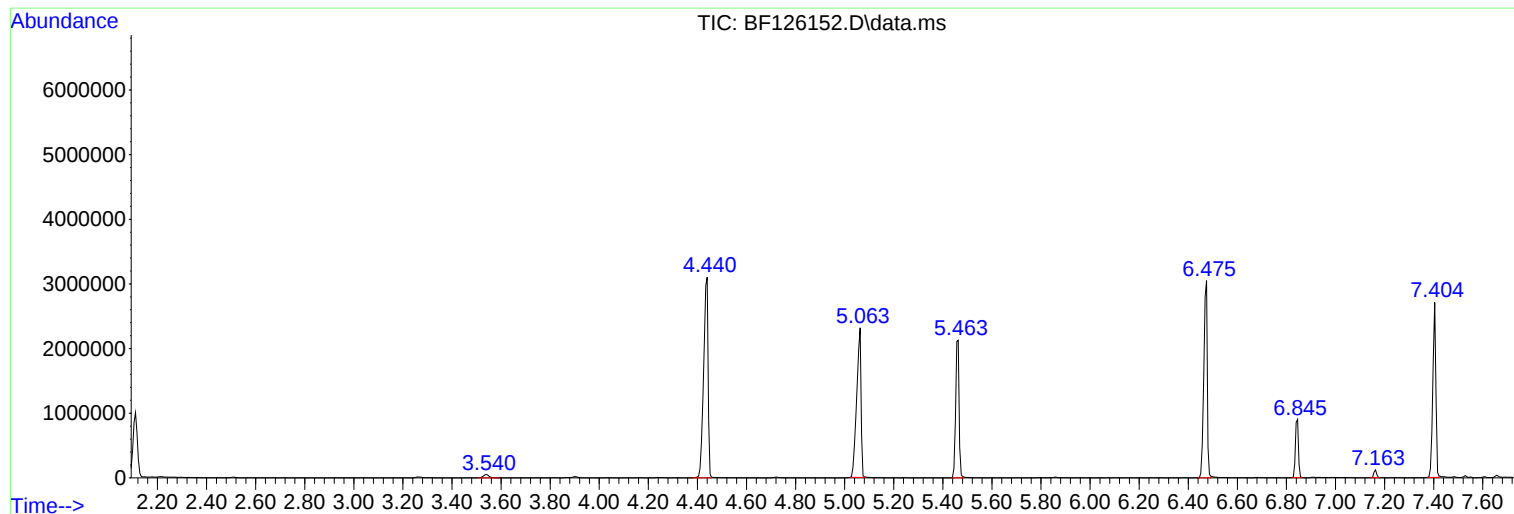

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
Data File : BF126152.D
Acq On : 12 Nov 2021 12:37
Operator : JU/CG
Sample : M4607-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
207

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
Data File : BF126152.D
Acq On : 12 Nov 2021 12:37
Operator : JU/CG
Sample : M4607-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
207

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------