


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
 Data File : BF126147.D
 Acq On : 12 Nov 2021 9:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 14:29:48 2021

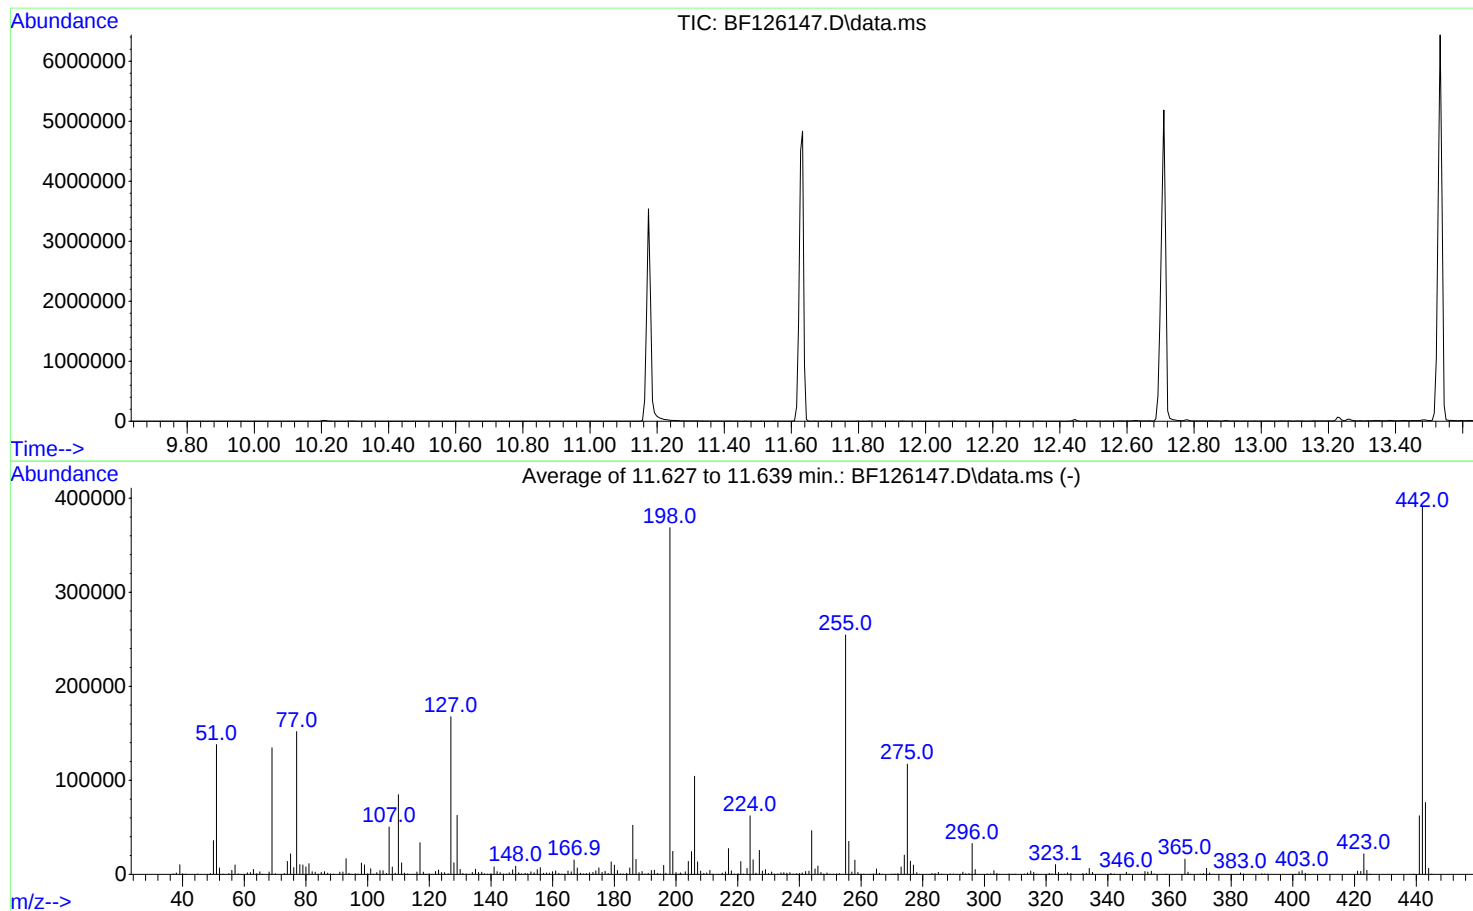




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	138057	PASS
68	69	0.00	2	2.0	2644	PASS
69	198	0.00	100	36.5	134645	PASS
70	69	0.00	2	0.6	765	PASS
127	198	10	80	45.5	167656	PASS
197	198	0.00	2	0.3	1279	PASS
198	198	100	100	100.0	368627	PASS
199	198	5	9	6.6	24509	PASS
275	198	10	60	31.8	117251	PASS
365	198	1	100	4.4	16194	PASS
441	198	0.01	100	16.9	62269	PASS
442	442	50	100	100.0	391168	PASS
443	442	15	24	19.5	76456	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
 Data File : BF126147.D
 Acq On : 12 Nov 2021 9:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 15 08:37:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 08:09:33 2021
 Response via : Initial Calibration

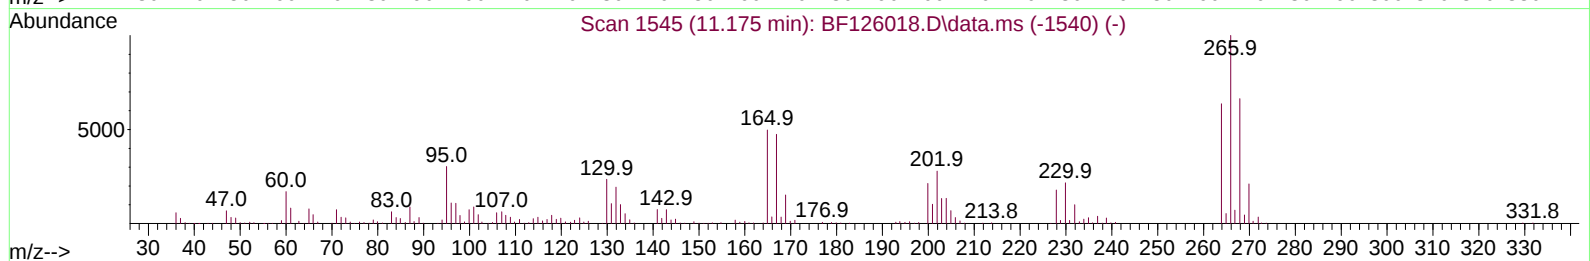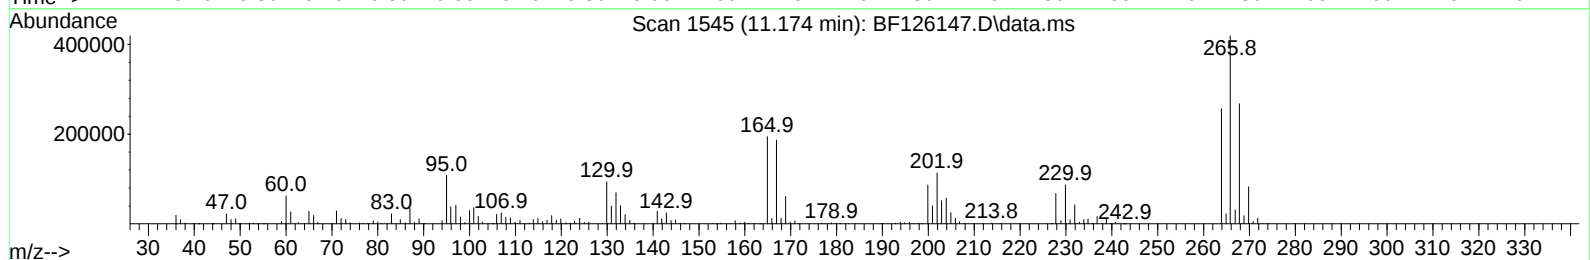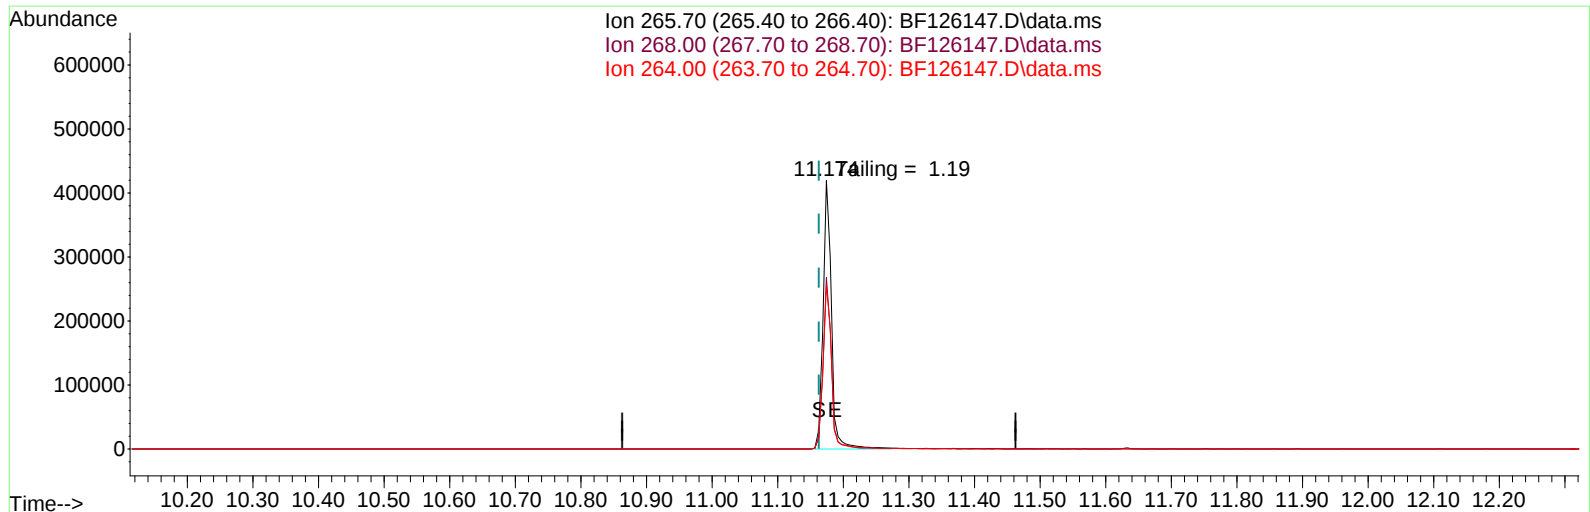

TIC: BF126147.D\data.ms

(70) Pentachlorophenol (C)

11.174min (+ 0.012) 25661.54 ng




response 373543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.84
264.00	69.90	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111221\
Data File : BF126147.D
Acq On : 12 Nov 2021 9:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 15 08:37:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 08:09:33 2021
Response via : Initial Calibration

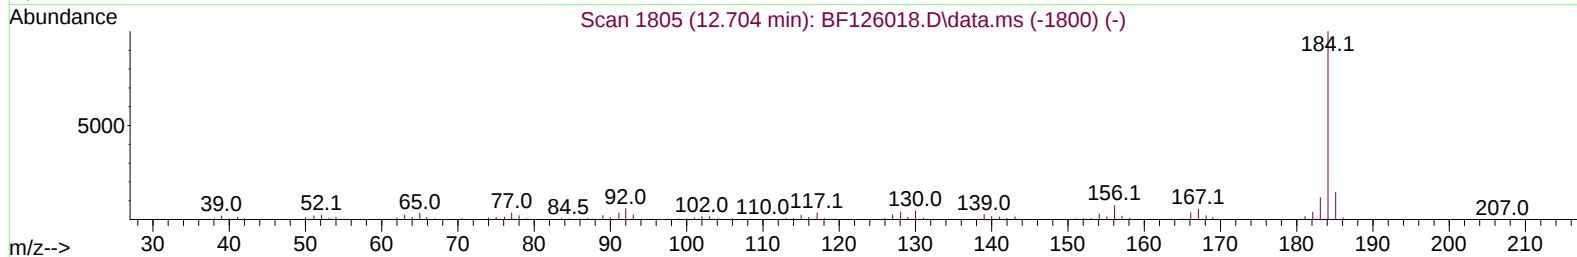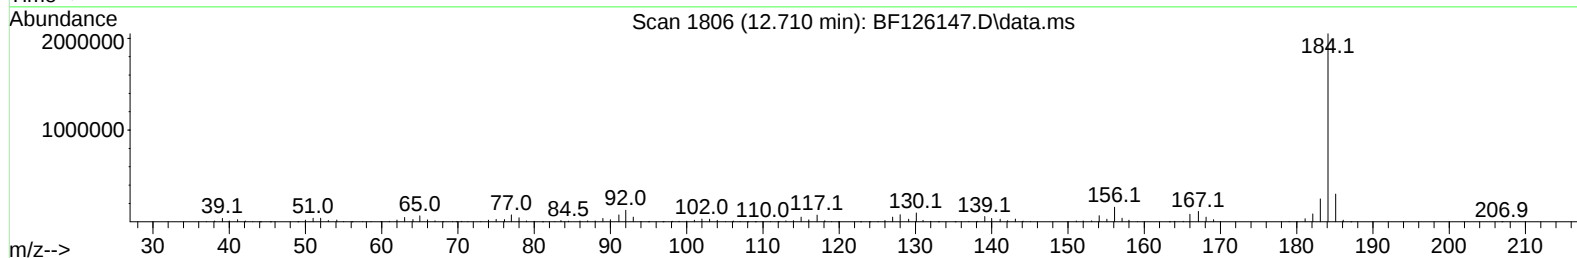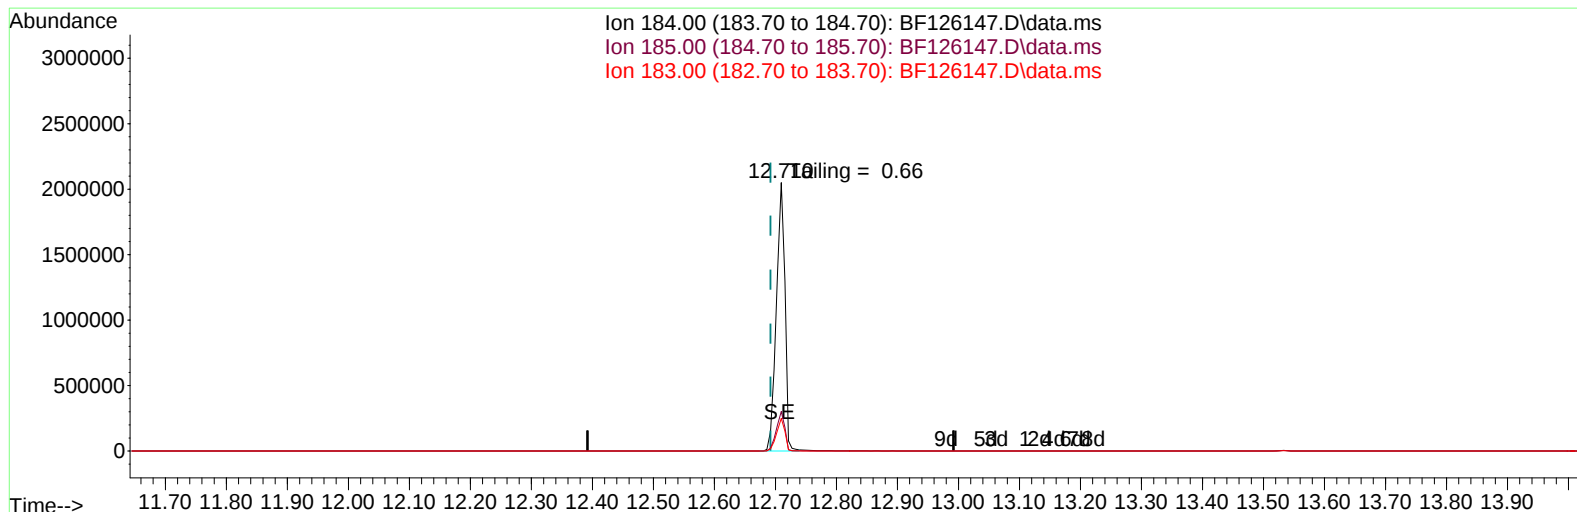

TIC: BF126147.D\data.ms

(77) Benzidine

12.710min (+ 0.017) 470308.37 ng m

response 2012406

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.74
183.00	10.10	12.19#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2021	BNA_F	<u>BF126147.D</u>
Compound Name	Response	Retention Time
DDT	1046848	13.568
DDD	18881	13.268
DDE	1470	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20351	1067199	1.91

Instrument :
BNA_F
ClientSampleId :
DFTPP