


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111318\
 Data File : BF110743.D
 Acq On : 14 Nov 2018 2:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 12:43:10 2018

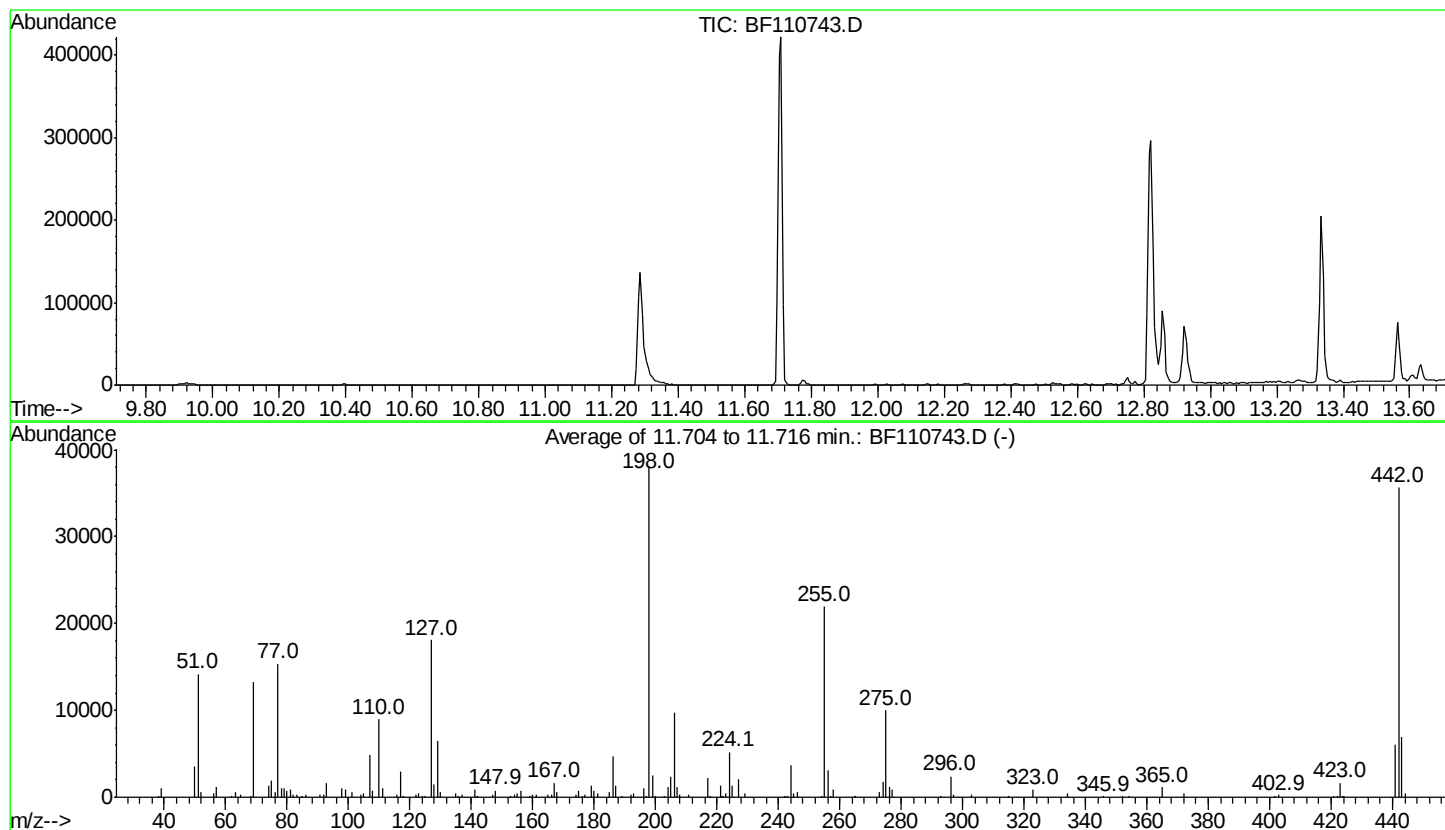

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	14151	PASS
68	69	0.00	2	1.3	179	PASS
69	198	0.00	100	34.9	13311	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	18081	PASS
197	198	0.00	2	0.5	195	PASS
198	198	100	100	100.0	38171	PASS
199	198	5	9	6.5	2477	PASS
275	198	10	60	26.1	9960	PASS
365	198	1	100	3.0	1164	PASS
441	198	0.01	100	16.0	6107	PASS
442	198	50	100	93.4	35634	PASS
443	442	15	24	19.5	6947	PASS