
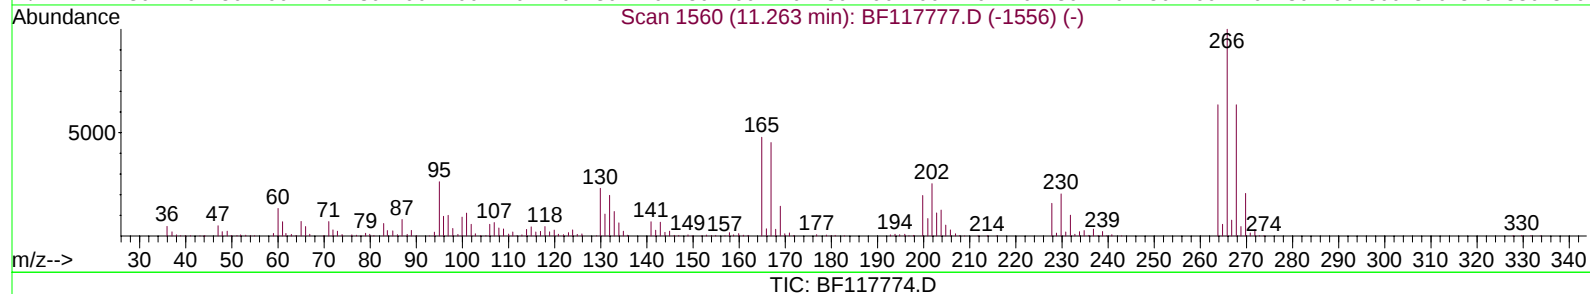
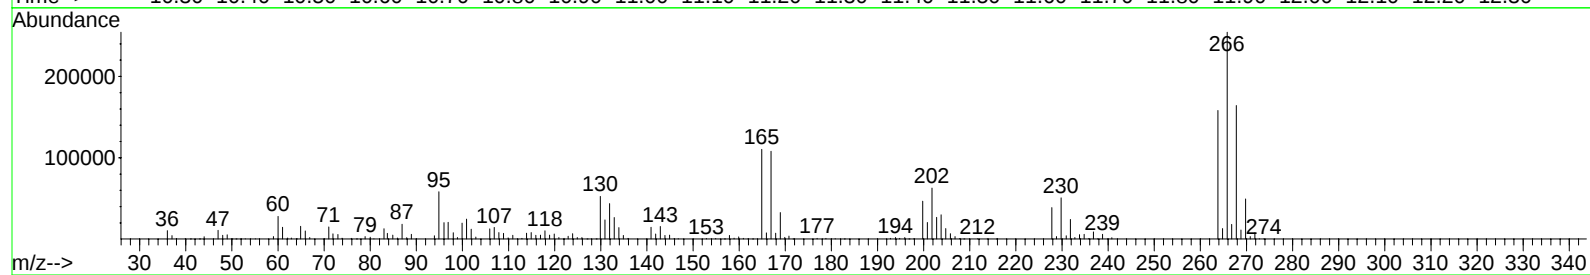


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111319\
Data File : BF117774.D
Acq On : 13 Nov 2019 14:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 17:31:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 16:36:34 2019
Response via : Initial Calibration

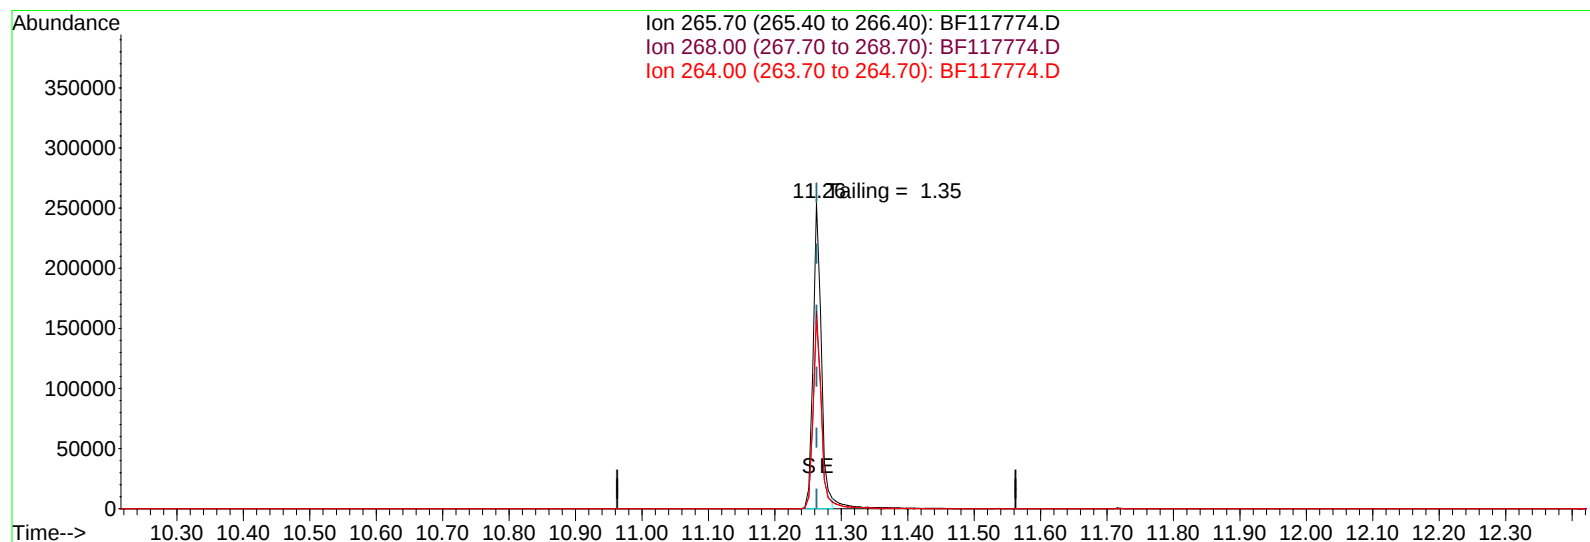

(70) Pentachlorophenol (C)




11.263min (-0.000) 34964.44ng

response 227854

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	64.59
264.00	63.40	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111319\
Data File : BF117774.D
Acq On : 13 Nov 2019 14:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 17:31:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 16:36:34 2019
Response via : Initial Calibration

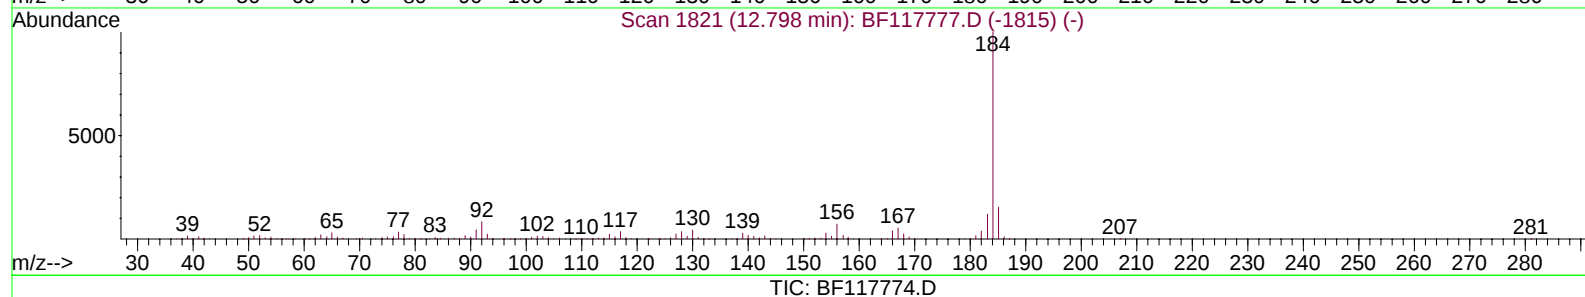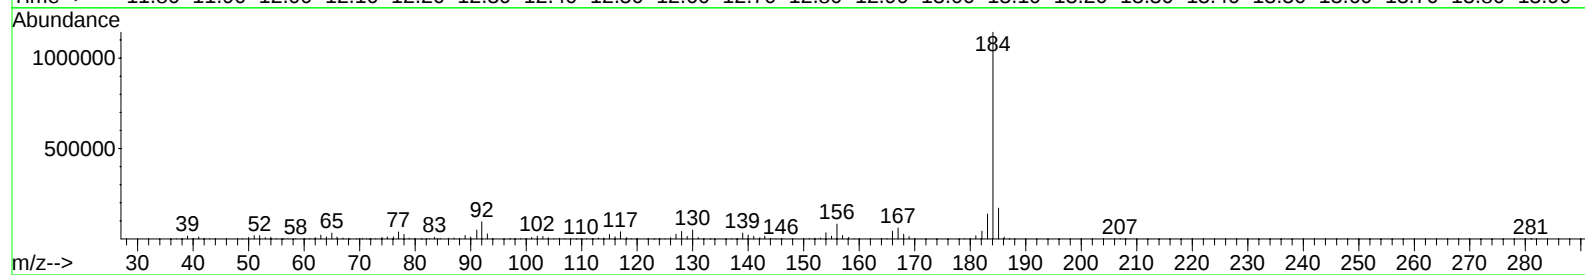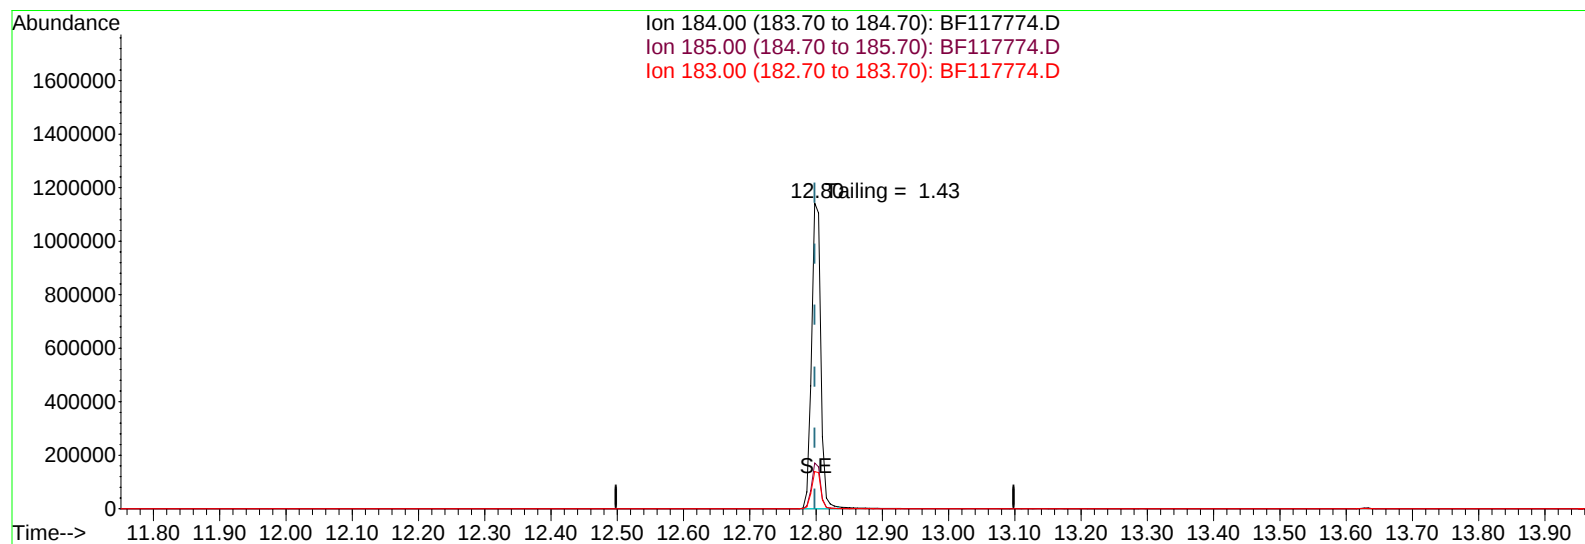

(77) Benzidine

12.798min (-0.000) 0.00ng

response 1114753

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.98
183.00	11.90	12.13
0.00	0.00	0.00