


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111319\
Data File : BF11774.D
Acq On : 13 Nov 2019 14:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 18:36:07 2019

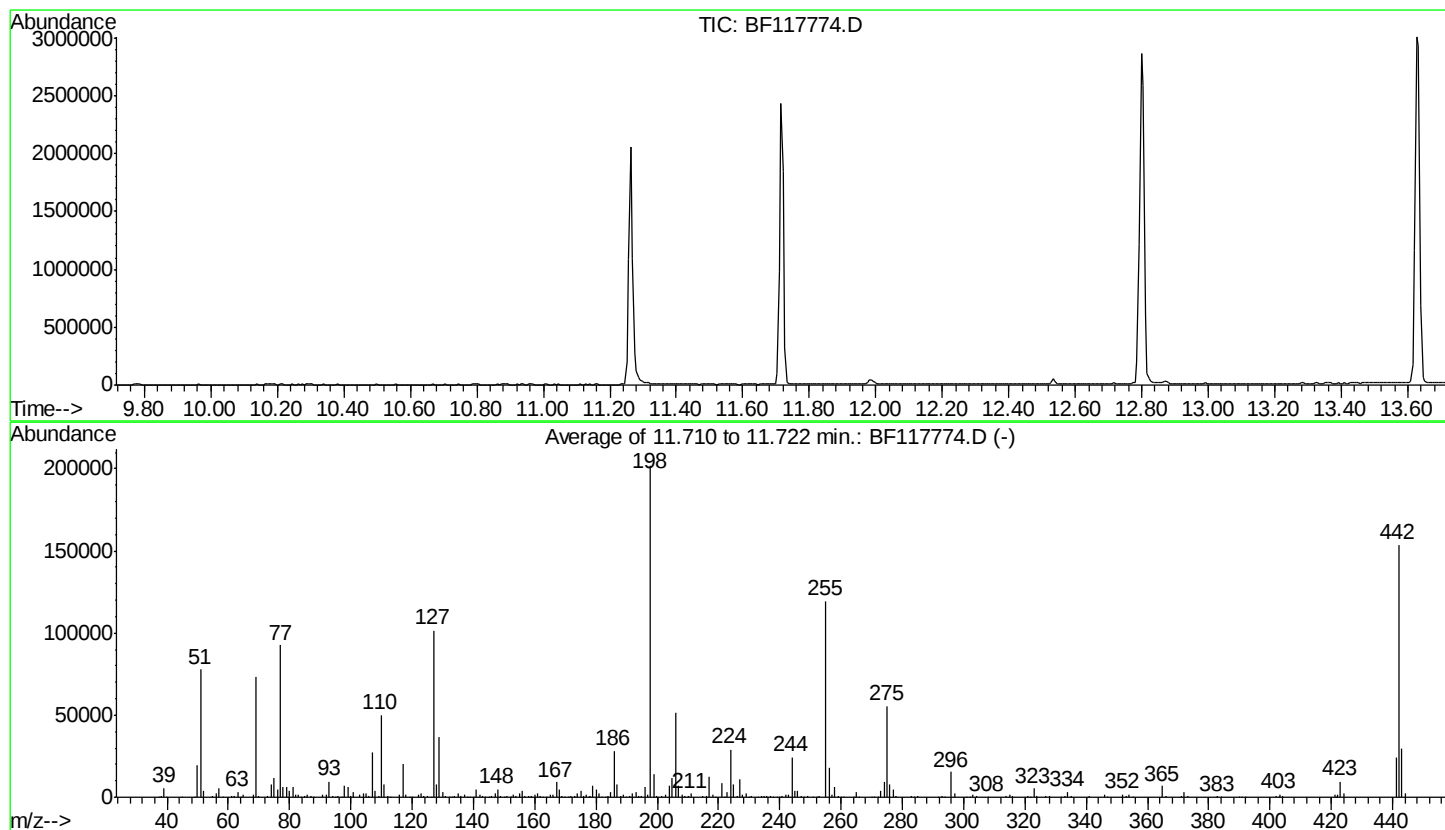

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	77657	PASS
68	69	0.00	2	1.8	1319	PASS
69	198	0.00	100	36.4	73480	PASS
70	69	0.00	2	0.6	437	PASS
127	198	10	80	50.2	101397	PASS
197	198	0.00	2	0.7	1432	PASS
198	198	100	100	100.0	201909	PASS
199	198	5	9	6.9	13967	PASS
275	198	10	60	27.6	55661	PASS
365	198	1	100	3.4	6858	PASS
441	198	0.01	100	12.2	24556	PASS
442	198	50	100	76.1	153717	PASS
443	442	15	24	19.2	29582	PASS