


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111320\
Data File : BF122324.D
Acq On : 13 Nov 2020 12:23
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 10 12:25:42 2020

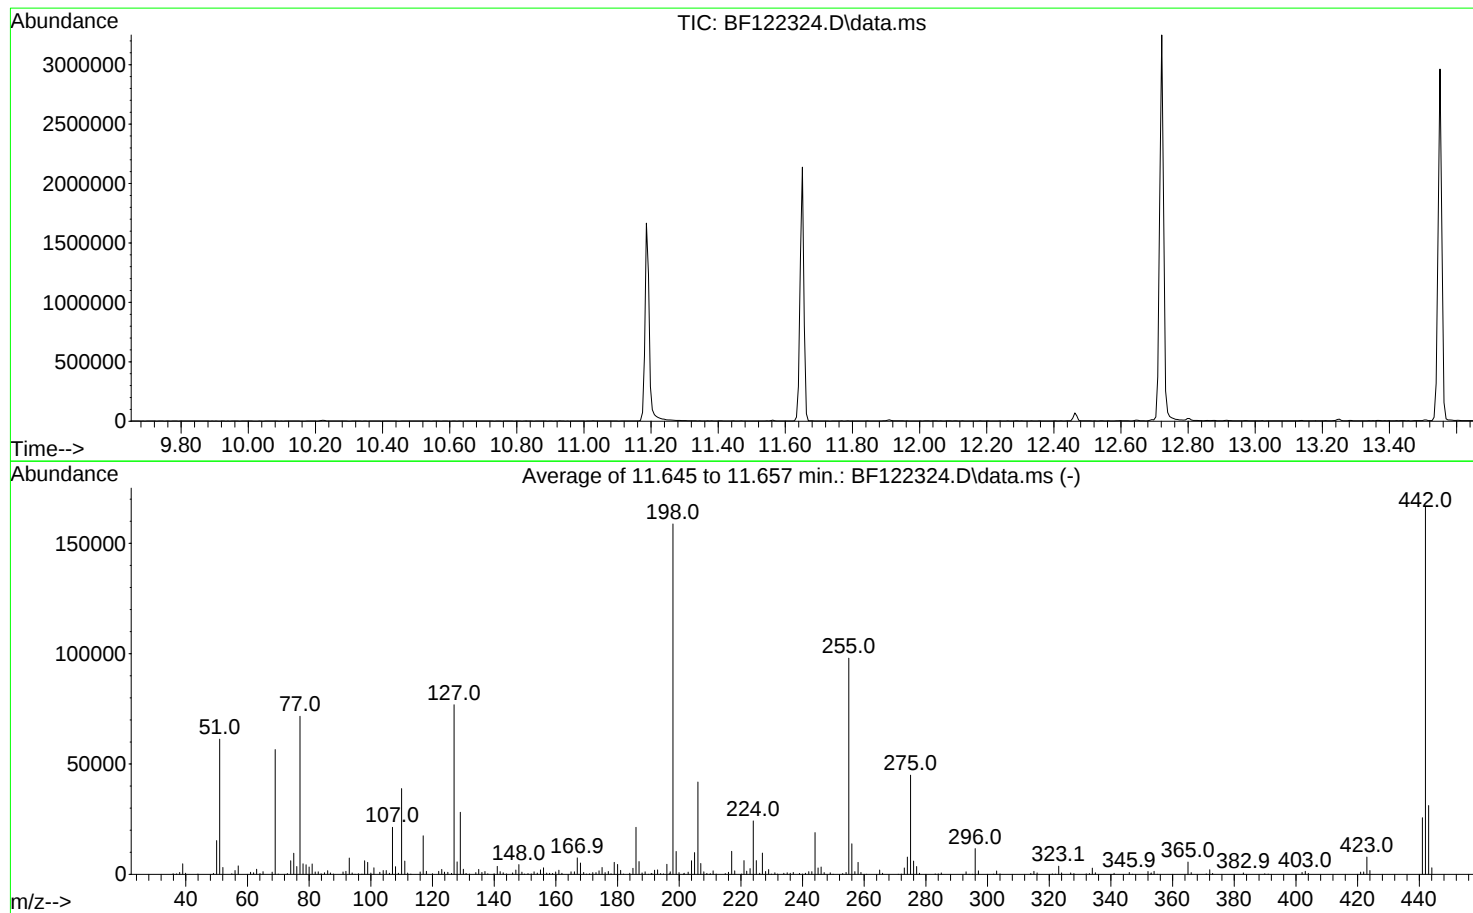

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	61277	PASS
68	69	0.00	2	1.8	994	PASS
69	198	0.00	100	35.6	56547	PASS
70	69	0.00	2	0.3	142	PASS
127	198	10	80	48.4	76853	PASS
197	198	0.00	2	0.7	1159	PASS
198	198	100	100	100.0	158819	PASS
199	198	5	9	6.5	10376	PASS
275	198	10	60	28.3	44928	PASS
365	198	1	100	3.5	5571	PASS
441	198	0.01	100	16.2	25674	PASS
442	442	100	100	100.0	166701	PASS
443	442	15	24	18.7	31163	PASS