
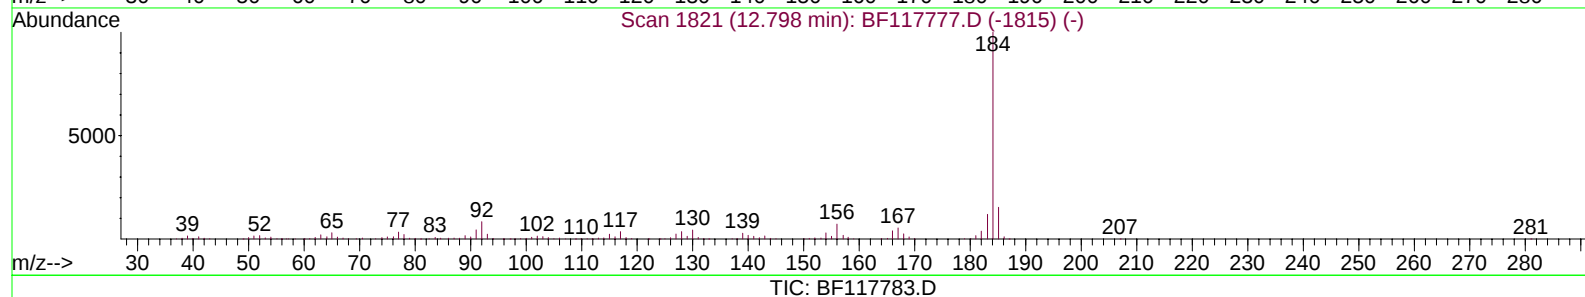
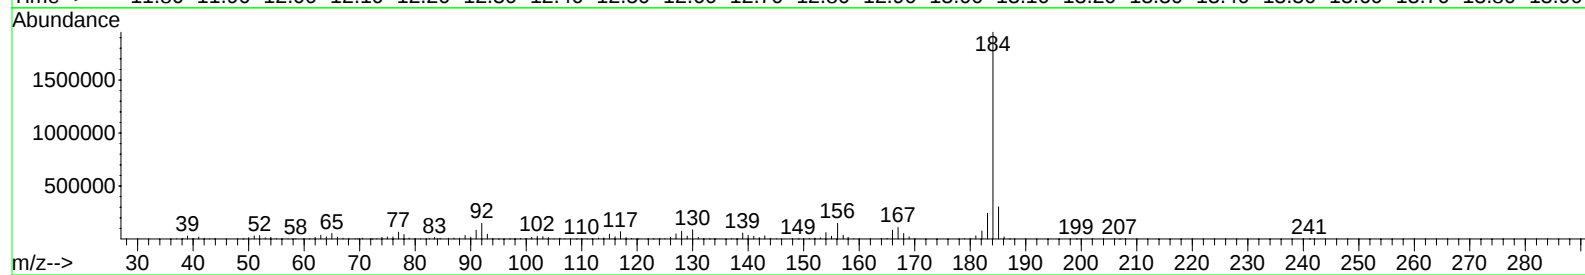


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111419\
Data File : BF117783.D
Acq On : 14 Nov 2019 8:49
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 18:10:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

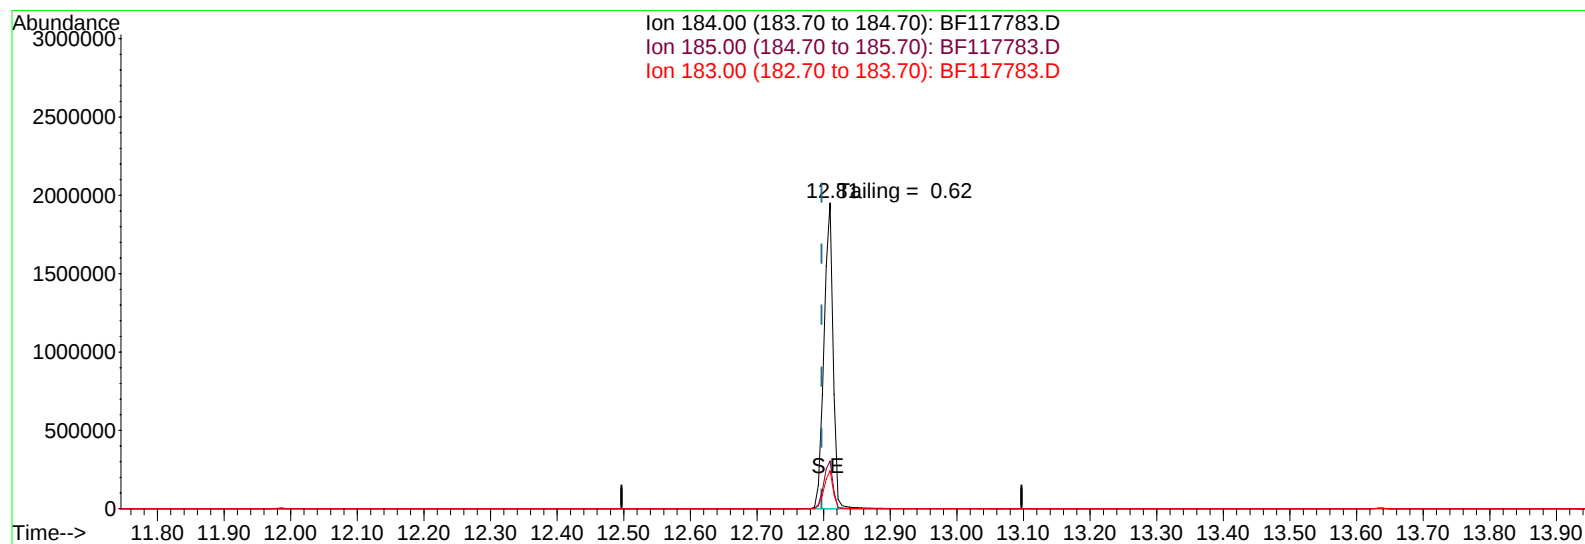

(77) Benzidine




12.810min (+0.013) 71064.43ng

response 1864548

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.59
183.00	11.90	12.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111419\
Data File : BF117783.D
Acq On : 14 Nov 2019 8:49
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 18:10:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

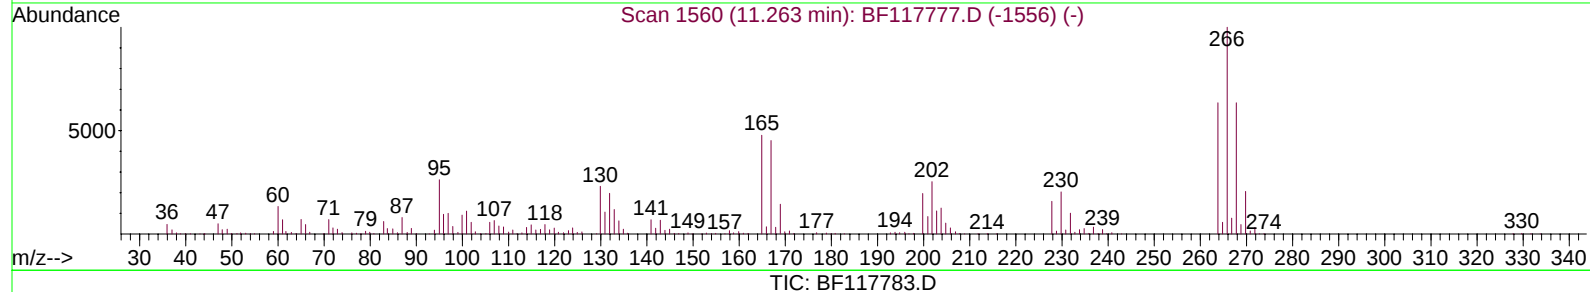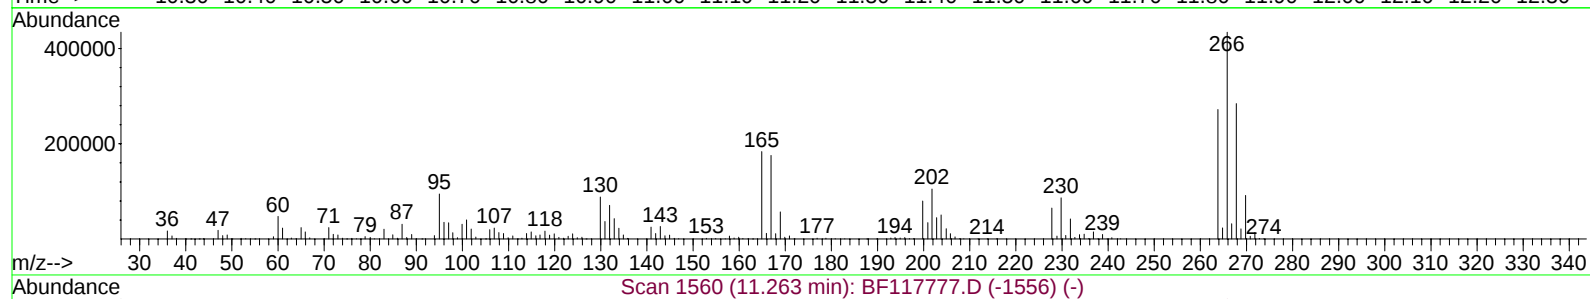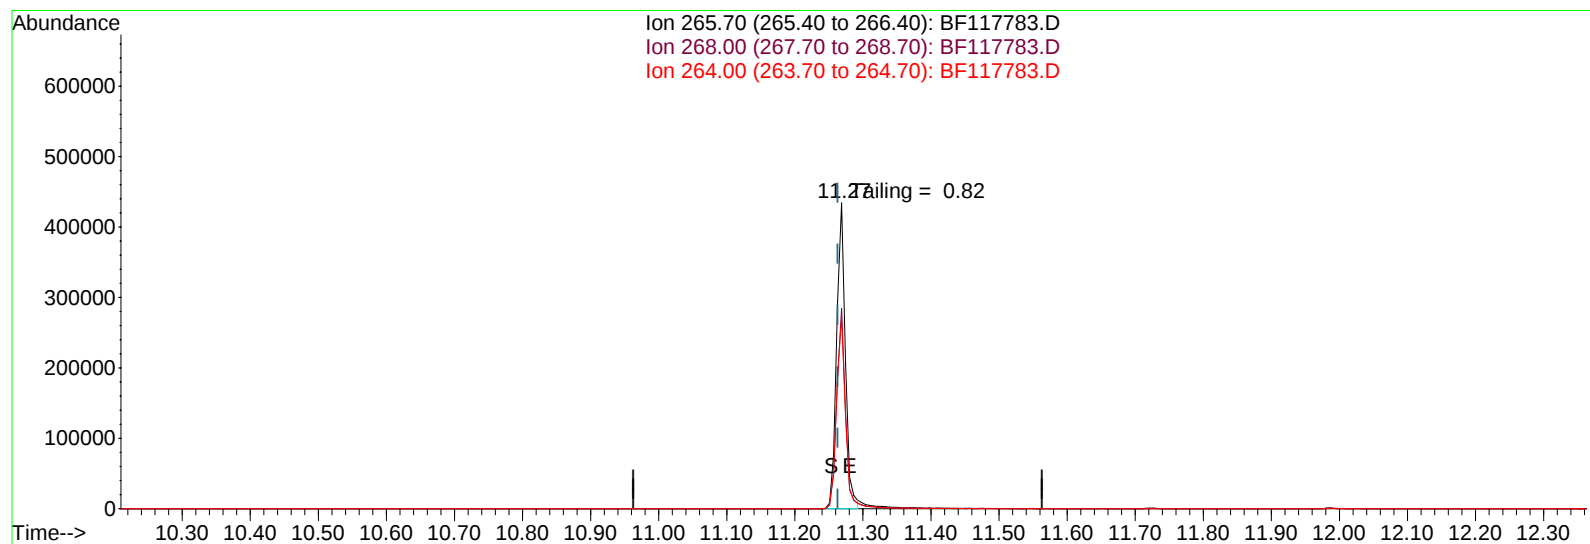

(70) Pentachlorophenol (C)

11.269min (+0.006) 53812.15ng

response 401876

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.55
264.00	63.40	62.66
0.00	0.00	0.00