


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111419\
 Data File : BF117783.D
 Acq On : 14 Nov 2019 8:49
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

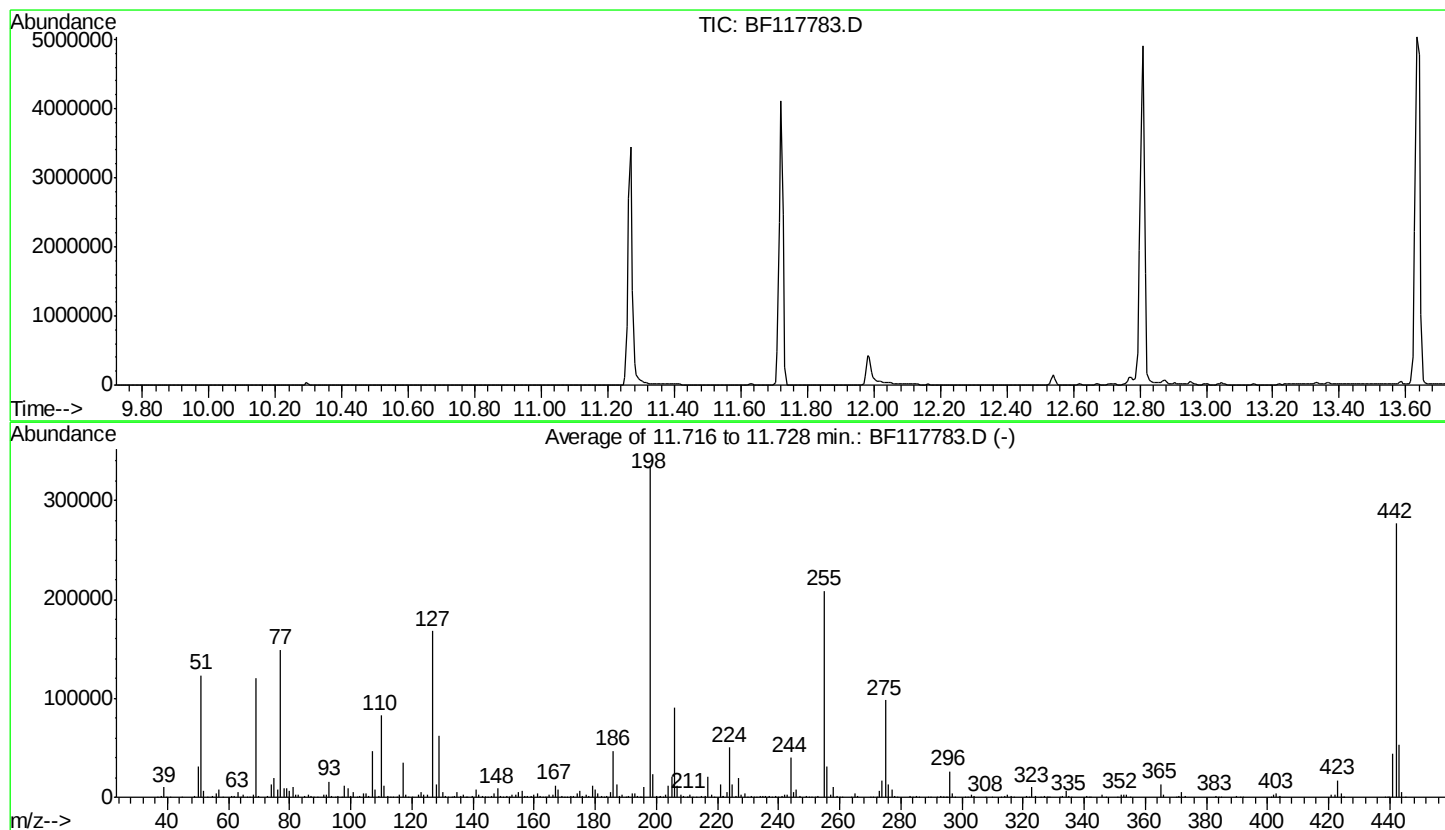

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	122973	PASS
68	69	0.00	2	1.9	2265	PASS
69	198	0.00	100	35.7	119853	PASS
70	69	0.00	2	0.7	784	PASS
127	198	10	80	50.1	168026	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	335296	PASS
199	198	5	9	6.9	23056	PASS
275	198	10	60	29.2	97925	PASS
365	198	1	100	3.9	12984	PASS
441	198	0.01	100	13.2	44413	PASS
442	198	50	100	82.5	276696	PASS
443	442	15	24	19.1	52832	PASS