


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111425\
Data File : BF144252.D
Acq On : 14 Nov 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

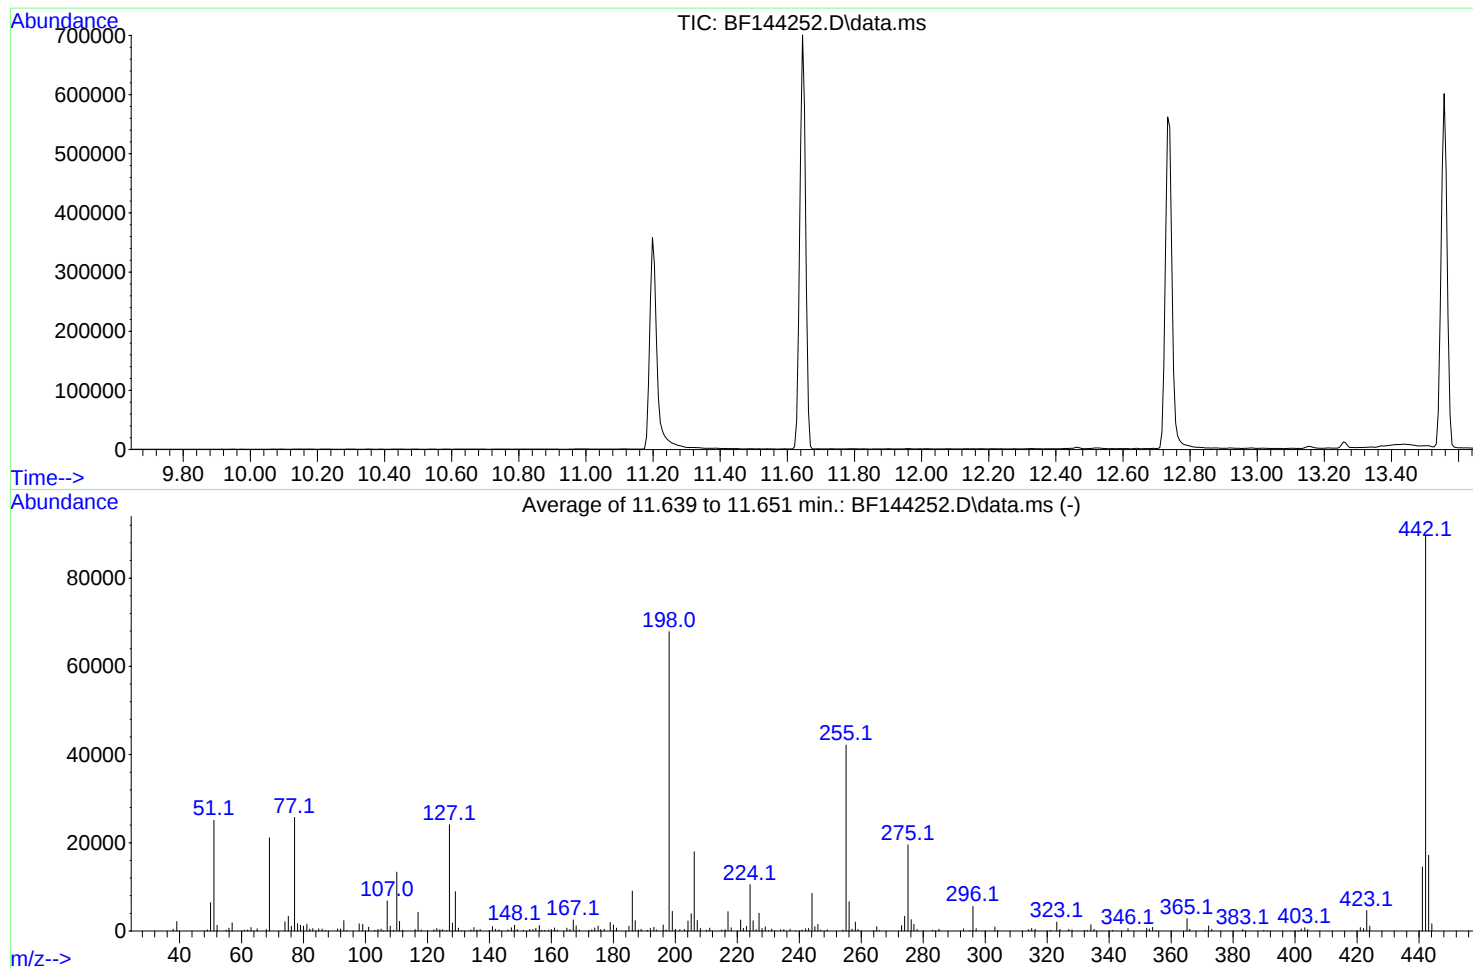

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	321	PASS
69	69	100	100	100.0	21117	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	257	PASS
198	198	100	100	100.0	67864	PASS
199	198	5	9	6.6	4480	PASS
365	198	1	100	4.1	2786	PASS
441	443	0.01	150	84.6	14537	PASS
442	442	100	100	100.0	89512	PASS
443	442	15	24	19.2	17176	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/14/2025	BNA_F	<u>BF144252.D</u>
Compound Name	Response	Retention Time
DDT	160686	13.557
DDD	4527	13.257
DDE	243	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4770	165456	2.88

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111425\
Data File : BF144252.D
Acq On : 14 Nov 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 14 09:49:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

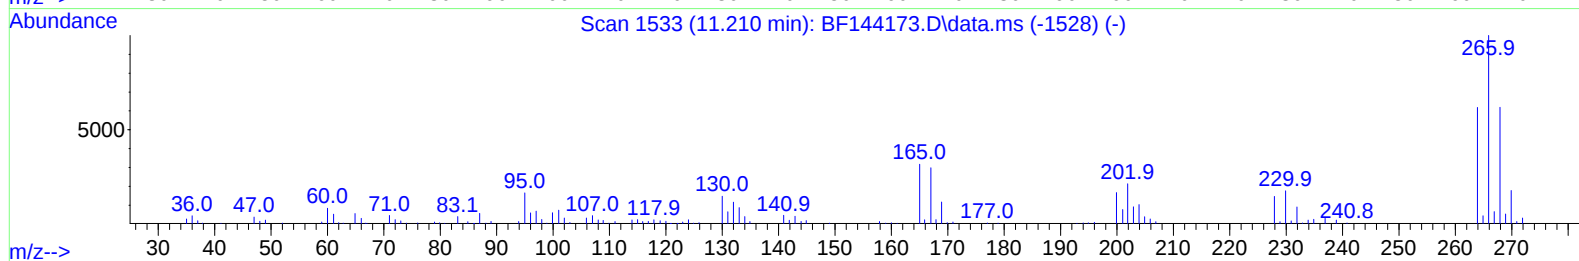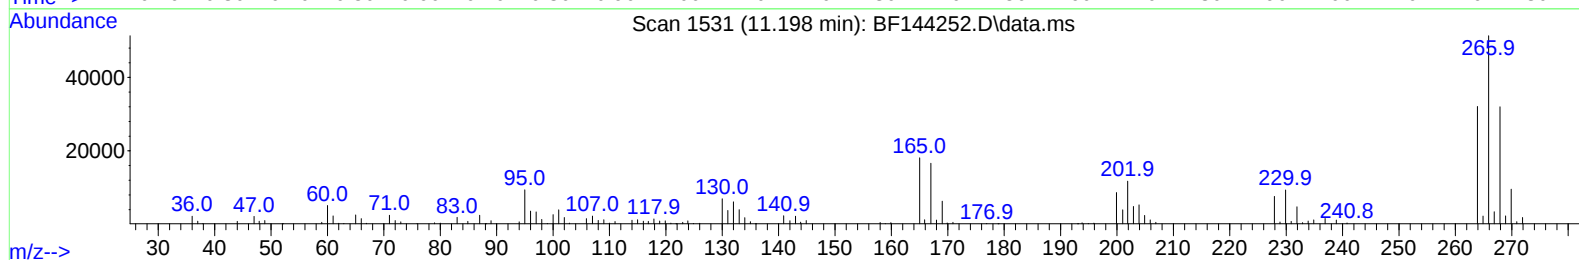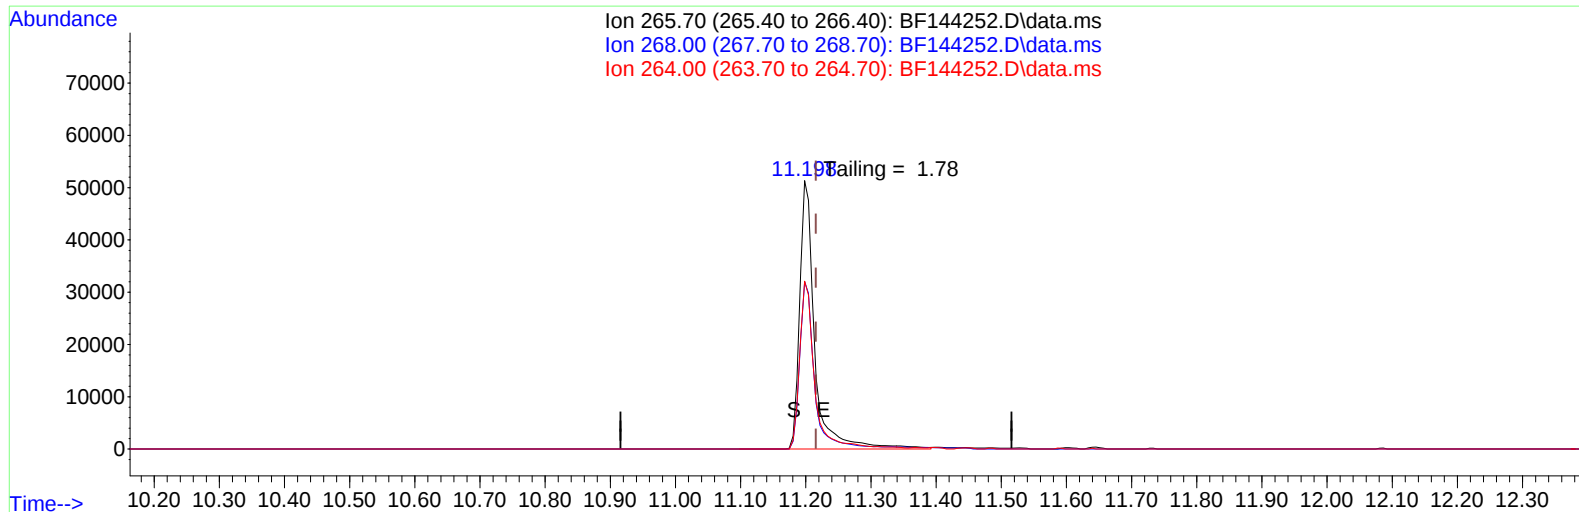

TIC: BF144252.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 38297.53 ng




response 82861

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.32
264.00	61.80	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111425\
Data File : BF144252.D
Acq On : 14 Nov 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 14 09:49:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

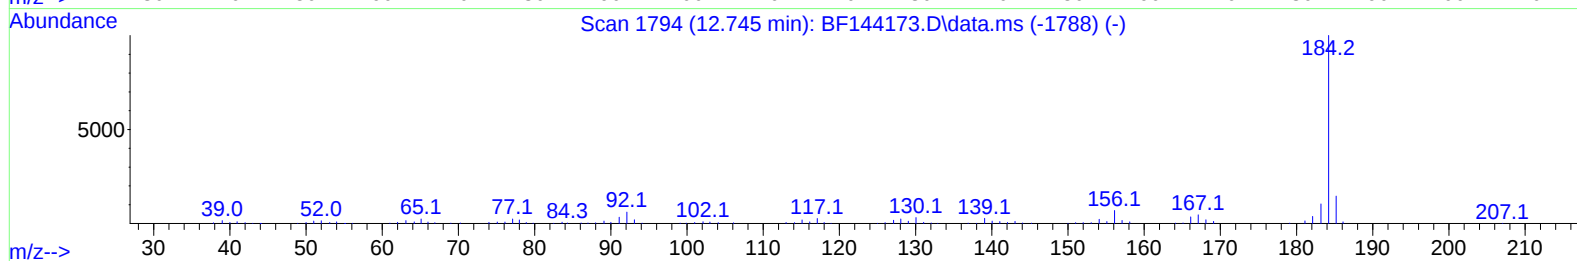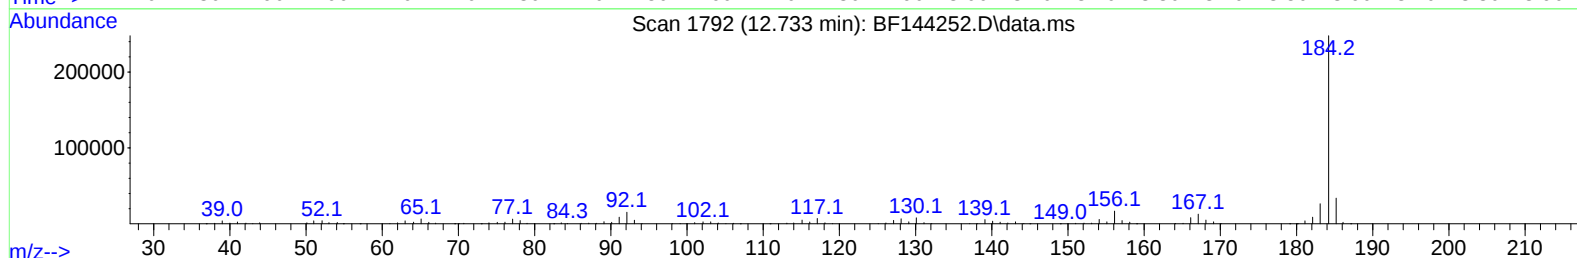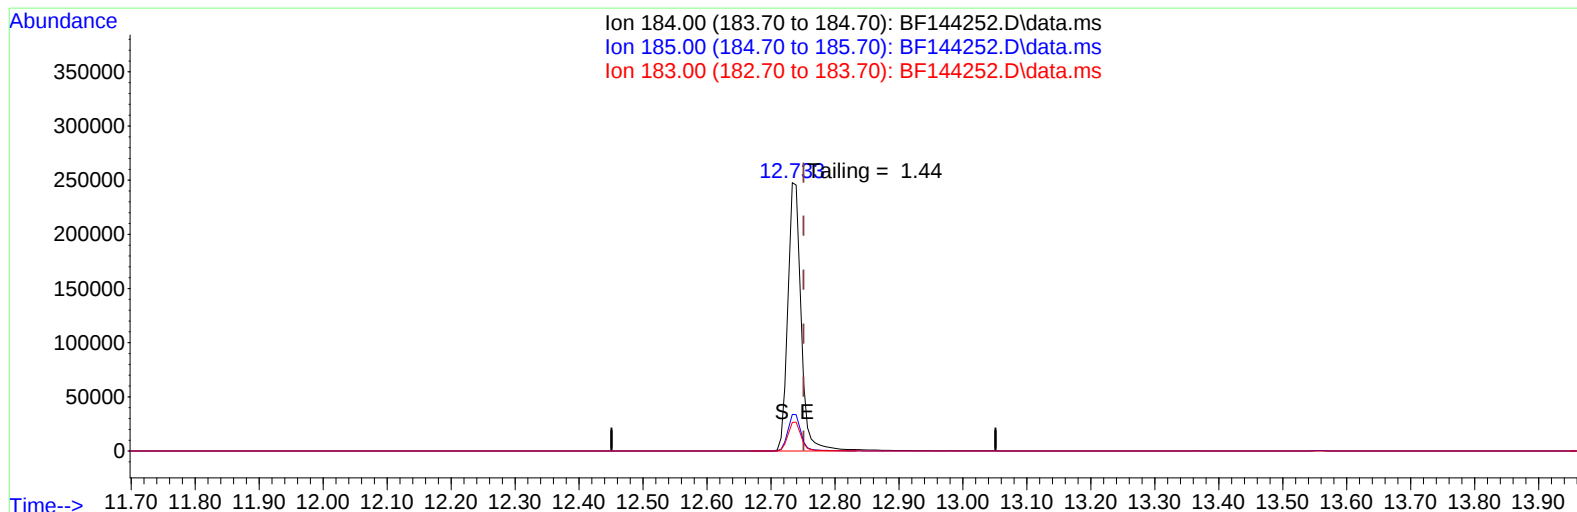

TIC: BF144252.D\data.ms

(77) Benzidine

12.733min (-0.018) 0.00 ng

response 359823

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.70
183.00	10.40	10.69
0.00	0.00	0.00