

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111518\
 Data File : BF110788.D
 Acq On : 15 Nov 2018 15:11
 Operator : JU/SJ
 Sample : J5950-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSI-21-TW-2

Quant Time: Nov 15 16:23:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.93	152	58083	20.00	ng	-0.01
21) Naphthalene-d8	8.22	136	238425	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	114973	20.00	ng	-0.01
64) Phenanthrene-d10	11.47	188	218558	20.00	ng	-0.01
76) Chrysene-d12	14.13	240	148277	20.00	ng	-0.01
87) Perylene-d12	15.66	264	139250	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	302078	84.48	ng	0.00
7) Phenol-d6	6.56	99	382075	83.56	ng	-0.01
23) Nitrobenzene-d5	7.50	82	232303	56.11	ng	-0.02
42) 2,4,6-Tribromophenol	10.77	330	98483	85.01	ng	-0.01
45) 2-Fluorobiphenyl	9.29	172	392950	48.81	ng	-0.01
79) Terphenyl-d14	13.06	244	401957	50.77	ng	-0.01
Target Compounds						
31) Naphthalene	8.25	128	28587	2.554	ng	99
50) Dimethylphthalate	9.69	163	62329	7.265	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111518\
Data File : BF110788.D
Acq On : 15 Nov 2018 15:11
Operator : JU/SJ
Sample : J5950-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SSI-21-TW-2

Quant Time: Nov 15 16:23:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

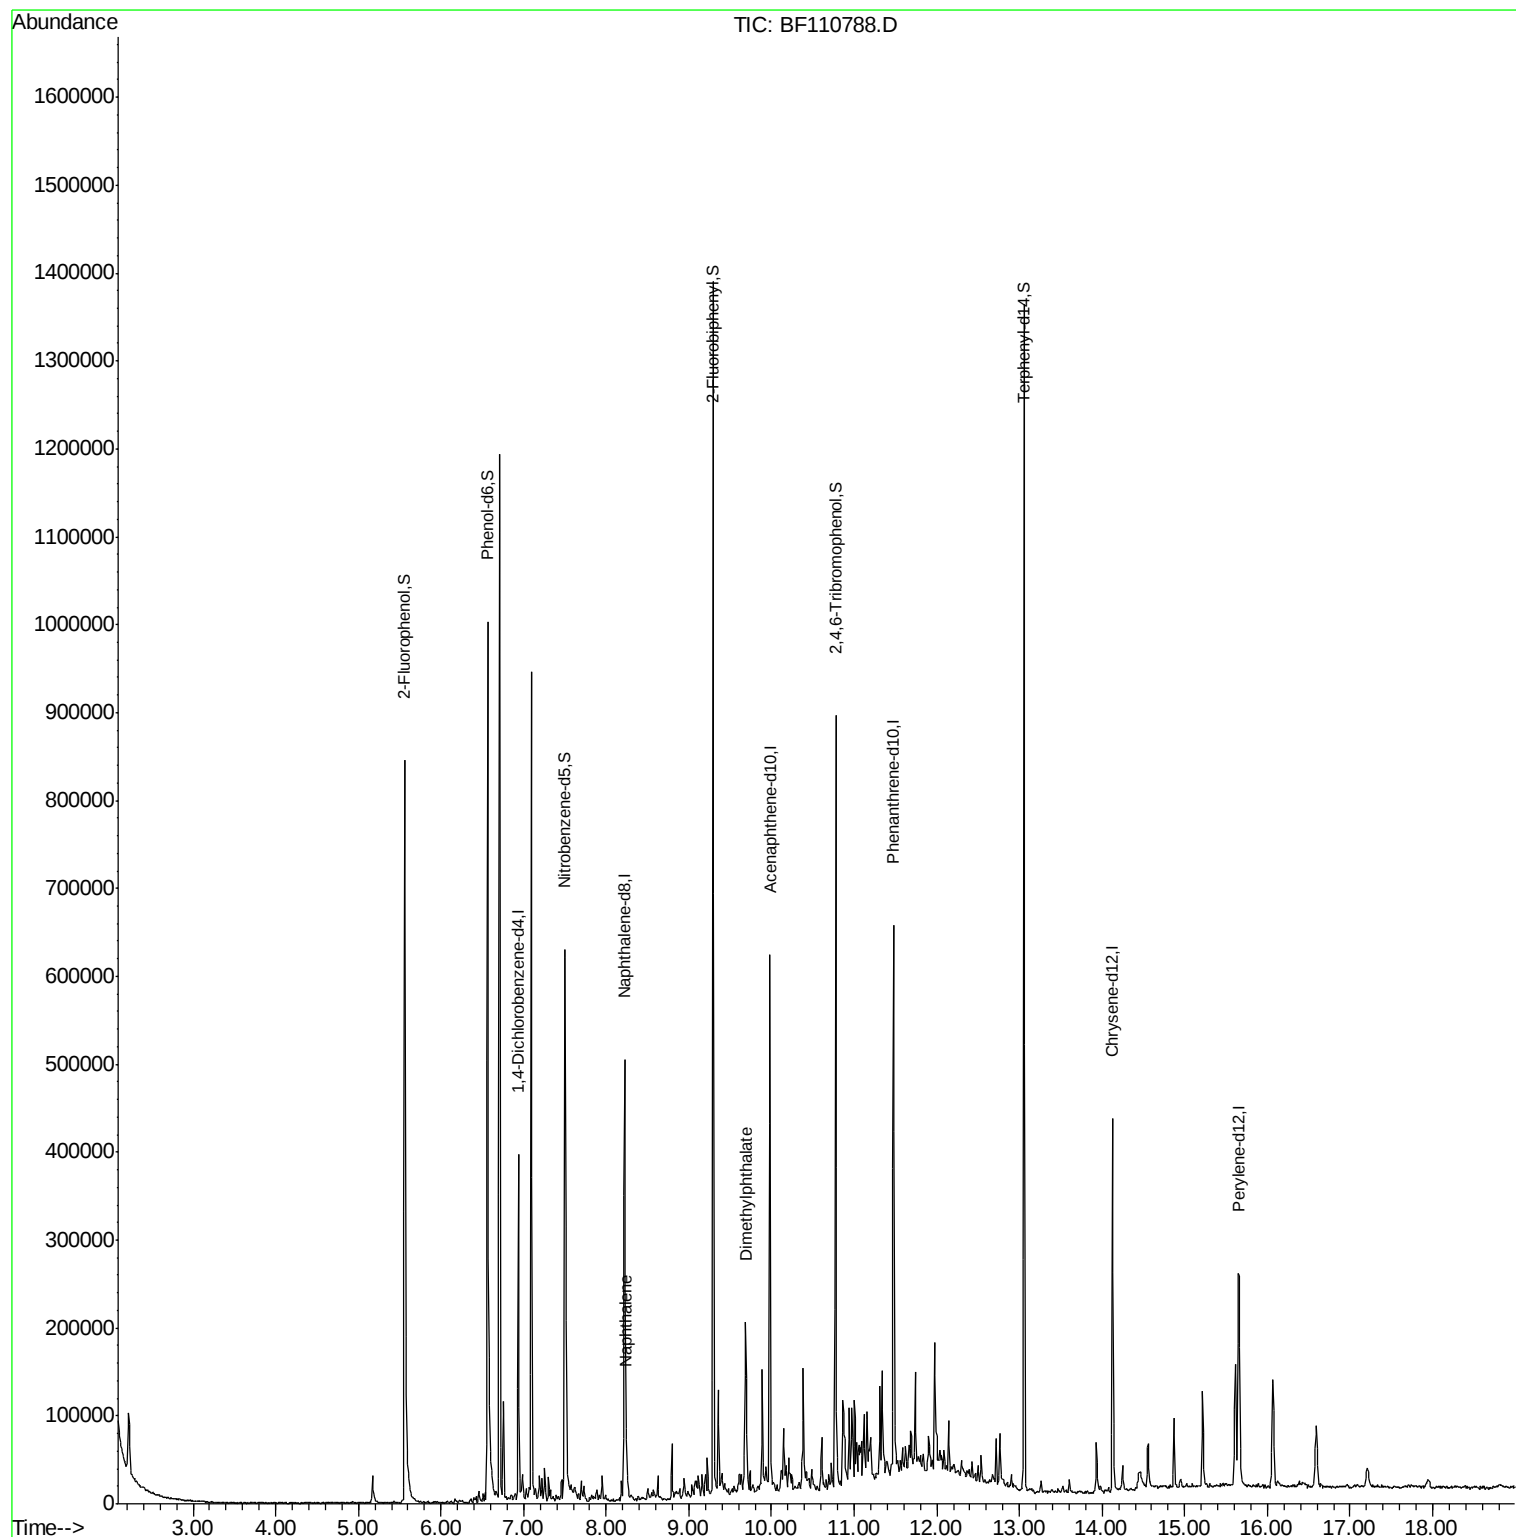

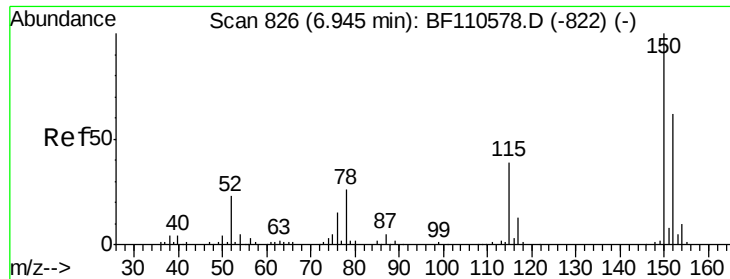


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.93 min Scan# 824
Delta R.T. -0.01 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11

Instrument :
BNA_F
ClientSampleId :
SSI-21-TW-2

Tgt Ion:152 Resp: 58083
Ion Ratio Lower Upper
152 100
150 160.2 122.7 184.1
115 67.5 49.1 73.7

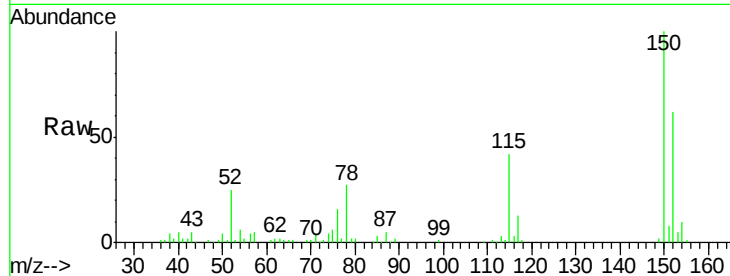


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

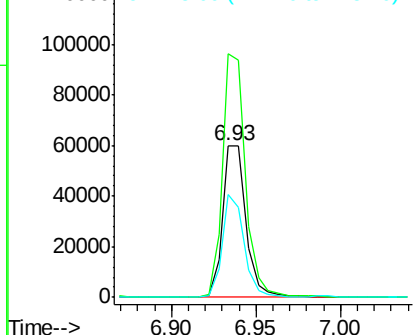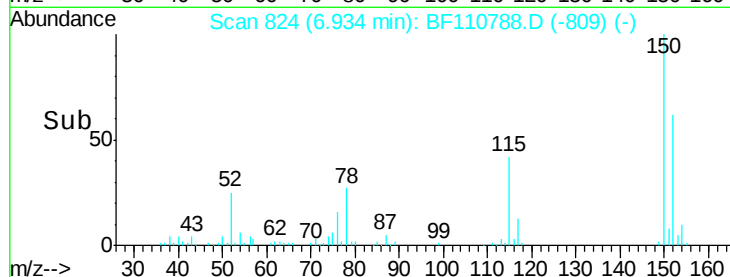



#5


2-Fluorophenol
Concen: 84.477 ng
RT: 5.56 min Scan# 590
Delta R.T. -0.01 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11

Tgt Ion:112 Resp: 302078
Ion Ratio Lower Upper
112 100
64 60.5 44.1 66.1
63 32.7 23.7 35.5

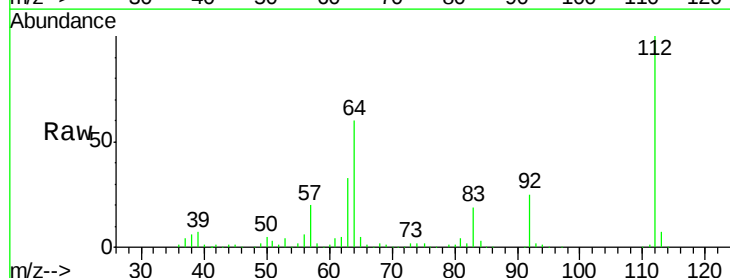

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

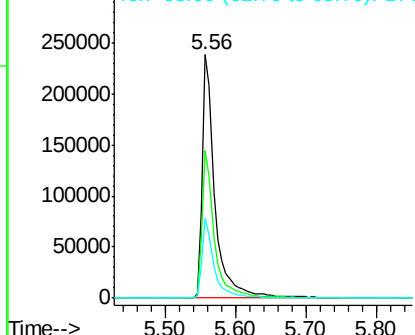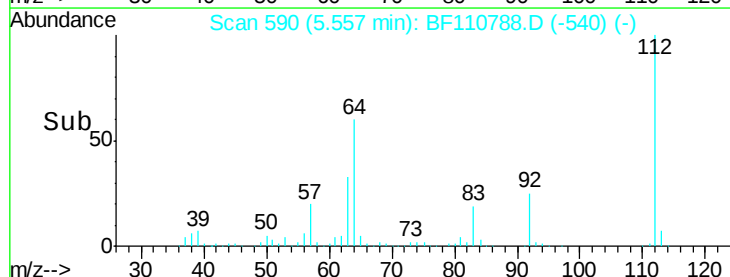

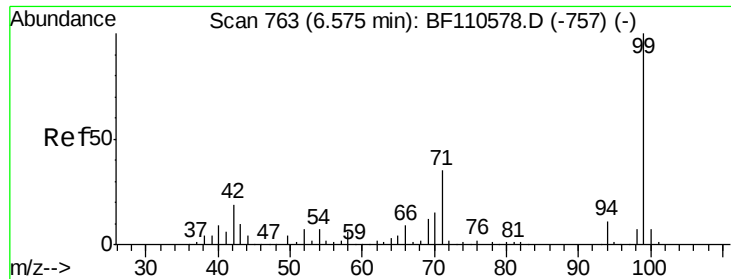

#7

Phenol-d6

Concen: 83.557 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110788.D

Acq: 15 Nov 2018 15:11

Instrument :

BNA_F

ClientSampleId :

SSI-21-TW-2


Tgt Ion: 99 Resp: 382075

Ion Ratio Lower Upper

99 100

42 19.4 15.8 23.6




71 35.2 28.0 42.0

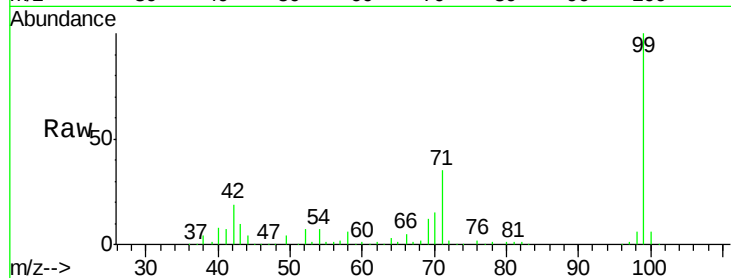

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

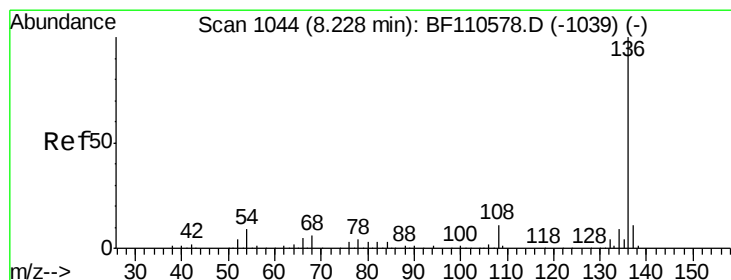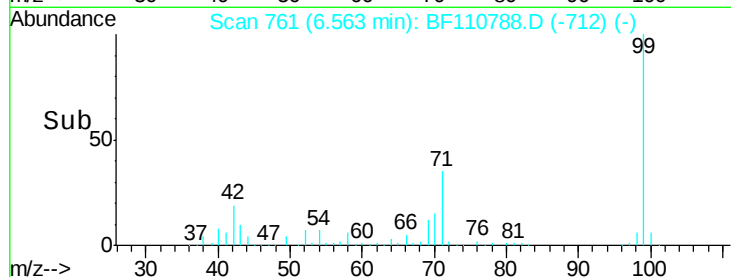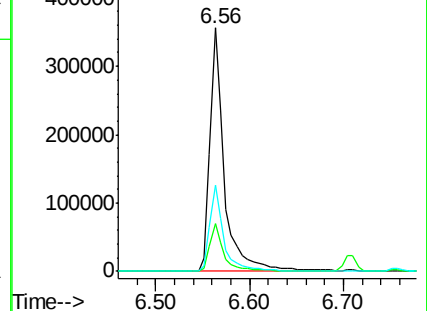

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.22 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF110788.D

Acq: 15 Nov 2018 15:11

Tgt Ion: 136 Resp: 238425


Ion Ratio Lower Upper

136 100

137 10.5 8.8 13.2

54 7.5 5.4 8.2

68 4.8 4.2 6.2


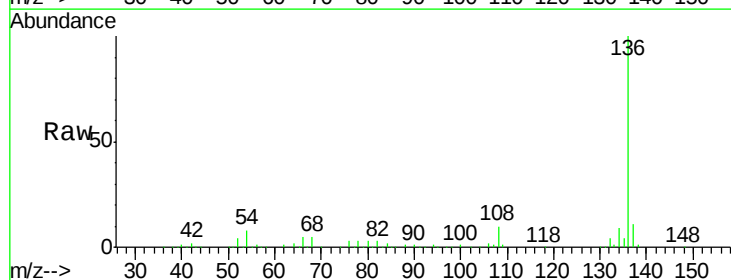



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



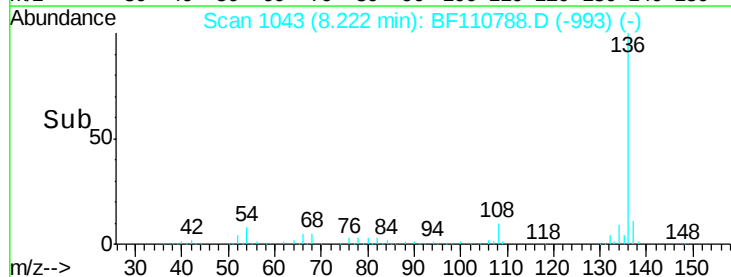
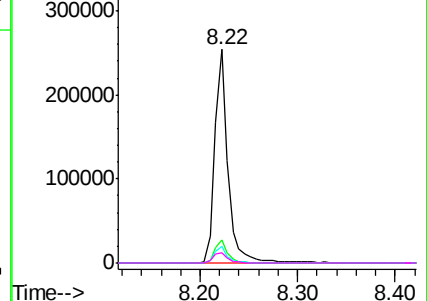


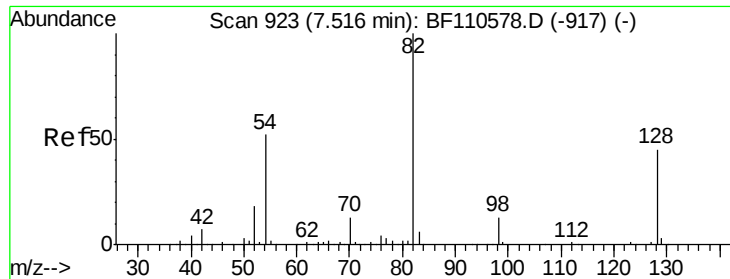

#23
Nitrobenzene-d5
Concen: 56.111 ng
RT: 7.50 min Scan# 920
Delta R.T. -0.02 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11




Instrument :
BNA_F
ClientSampleId :
SSI-21-TW-2


Tgt Ion: 82 Resp: 232303
Ion Ratio Lower Upper
82 100
128 43.3 34.2 51.2
54 54.8 38.6 58.0

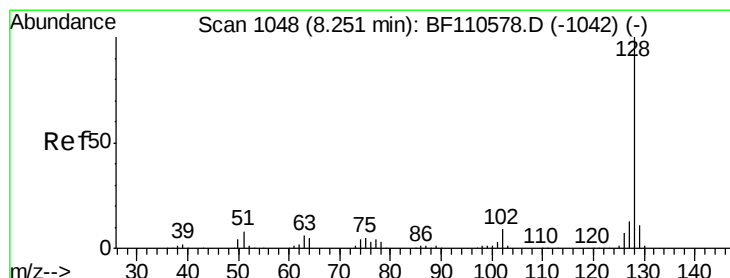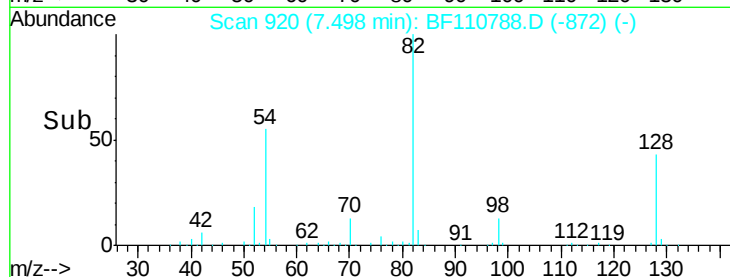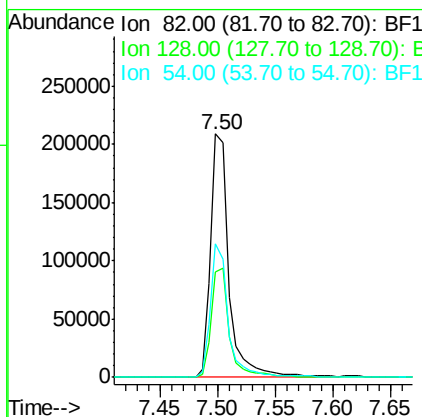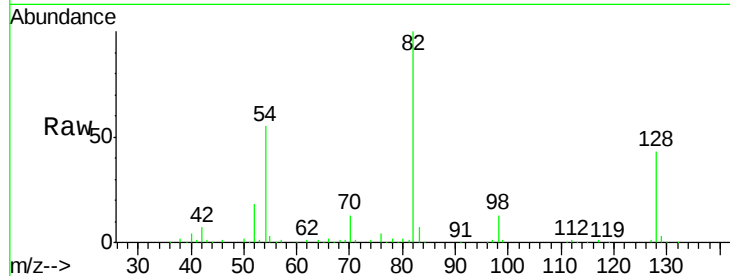

#31
Naphthalene
Concen: 2.554 ng
RT: 8.25 min Scan# 1047
Delta R.T. -0.01 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11

Tgt Ion: 128 Resp: 28587
Ion Ratio Lower Upper
128 100
129 9.9 8.8 13.2
127 13.6 10.8 16.2


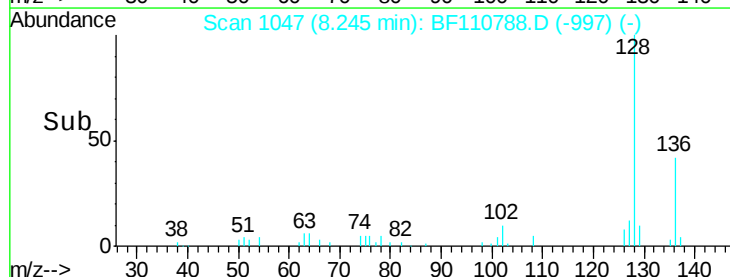
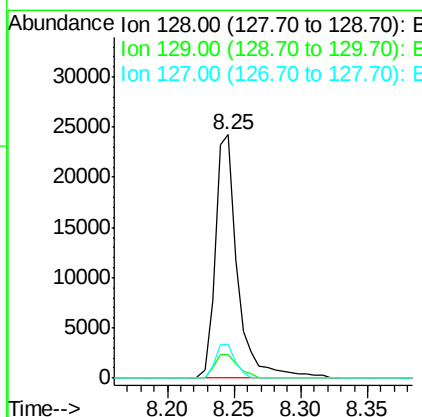
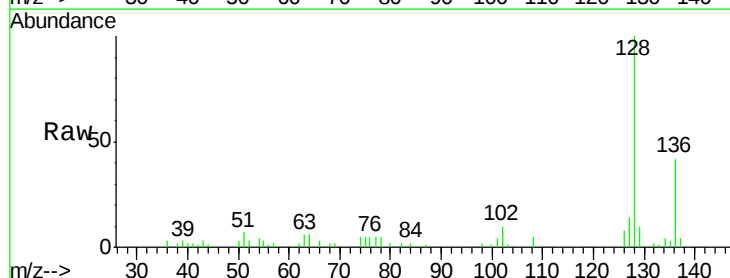


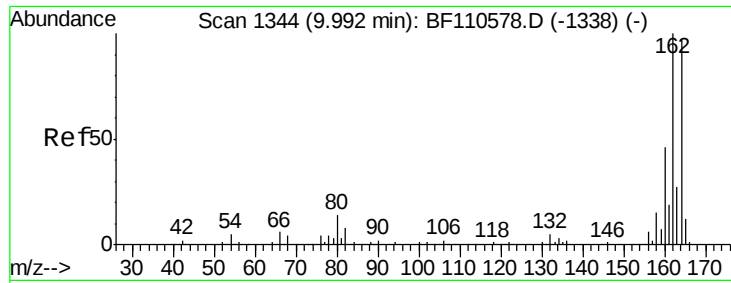

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.98 min Scan# 1342
 Delta R.T. -0.01 min
 Lab File: BF110788.D
 Acq: 15 Nov 2018 15:11




Instrument :
 BNA_F
 ClientSampleId :
 SSI-21-TW-2


Tgt Ion:164 Resp: 114973
 Ion Ratio Lower Upper
 164 100
 162 105.0 83.0 124.6
 160 47.0 37.0 55.6

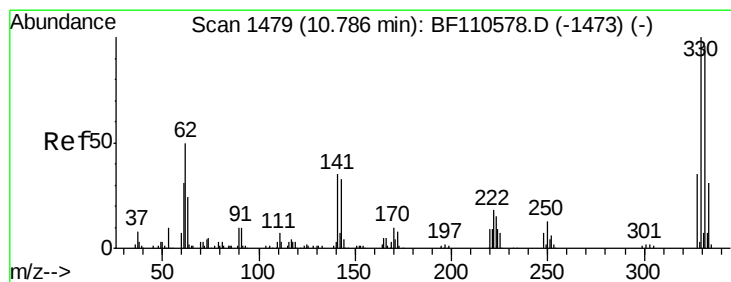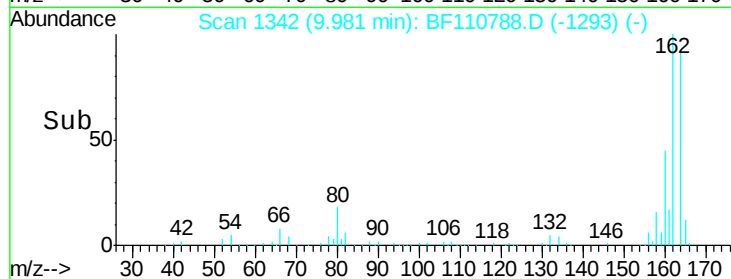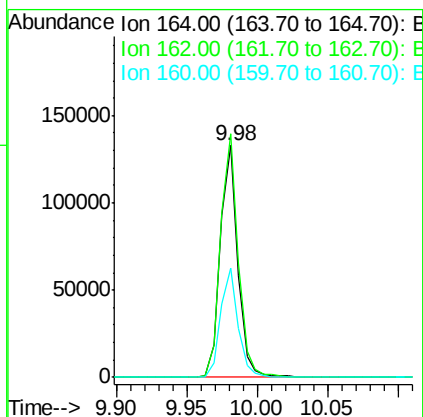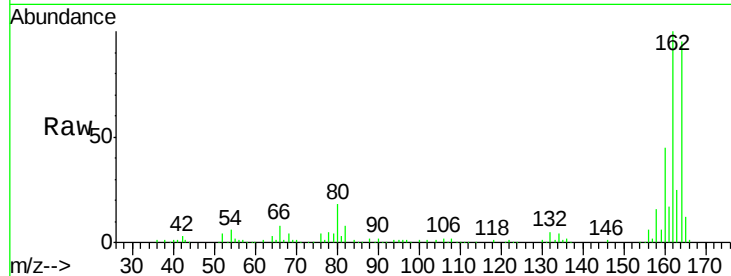

#42
 2,4,6-Tribromophenol
 Concen: 85.009 ng
 RT: 10.77 min Scan# 1477
 Delta R.T. -0.01 min
 Lab File: BF110788.D
 Acq: 15 Nov 2018 15:11

Tgt Ion:330 Resp: 98483
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.1 115.7
 141 38.3 27.0 40.4

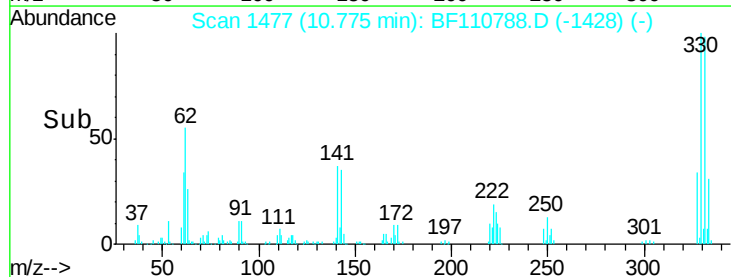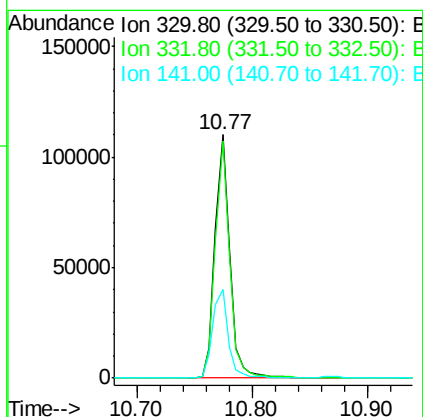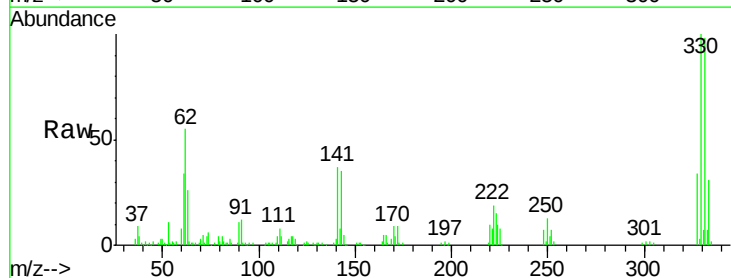


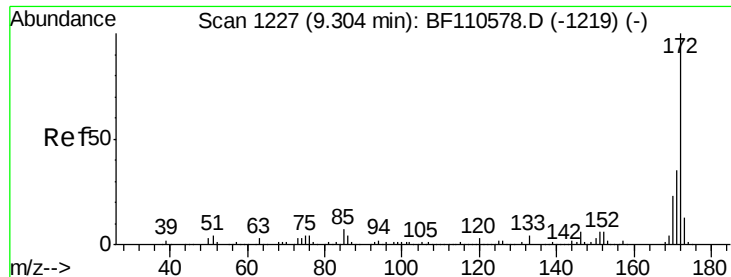




#45
 2-Fluorobiphenyl
 Concen: 48.812 ng
 RT: 9.29 min Scan# 1225
 Delta R.T. -0.01 min
 Lab File: BF110788.D
 Acq: 15 Nov 2018 15:11

Instrument :
 BNA_F
 ClientSampleId :
 SSI-21-TW-2

Tgt Ion:172 Resp: 392950
 Ion Ratio Lower Upper
 172 100
 171 34.5 28.6 43.0
 170 22.9 19.7 29.5

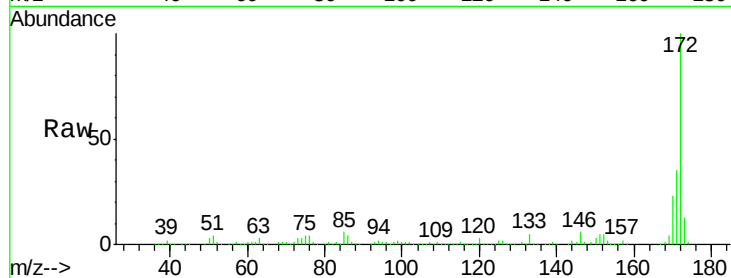


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

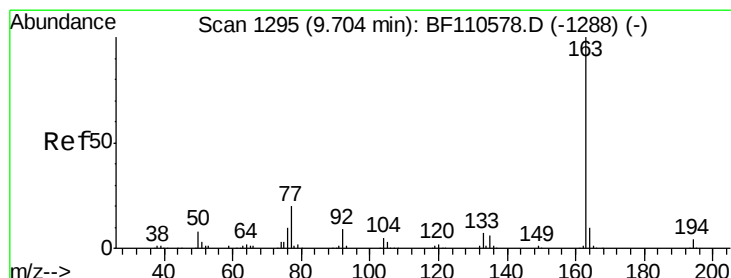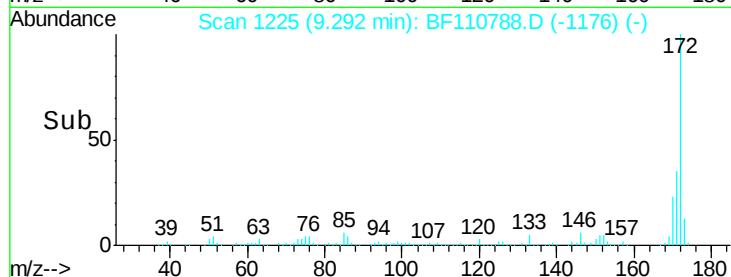
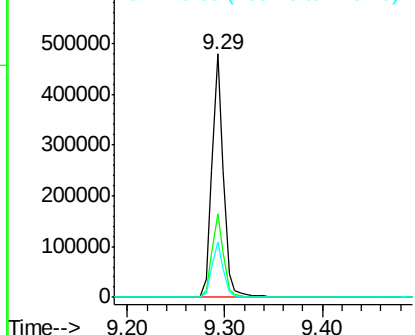



#50
 Dimethylphthalate
 Concen: 7.265 ng
 RT: 9.69 min Scan# 1292
 Delta R.T. -0.02 min
 Lab File: BF110788.D
 Acq: 15 Nov 2018 15:11

Tgt Ion:163 Resp: 62329
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.2 4.8
 164 9.9 8.1 12.1

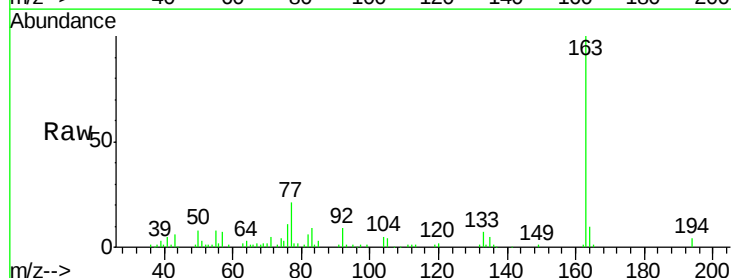

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



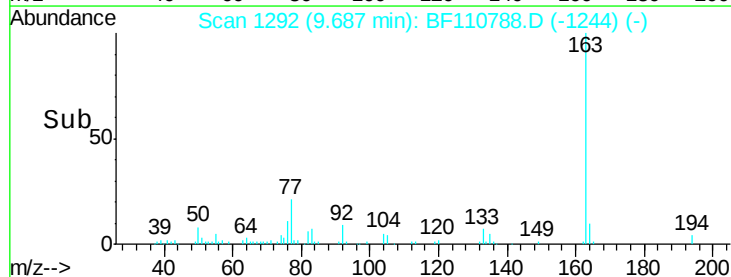
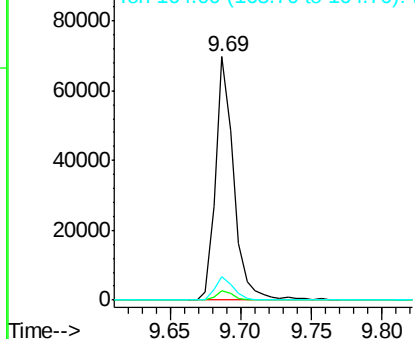


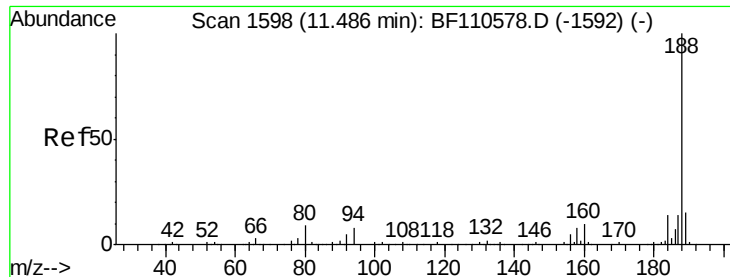

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.47 min Scan# 1596
Delta R.T. -0.01 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11




Instrument :
BNA_F
ClientSampleId :
SSI-21-TW-2


Tgt Ion	Ratio	Resp	Lower	Upper
188	100	218558		
94	9.1		7.2	10.8
80	9.7		7.9	11.9

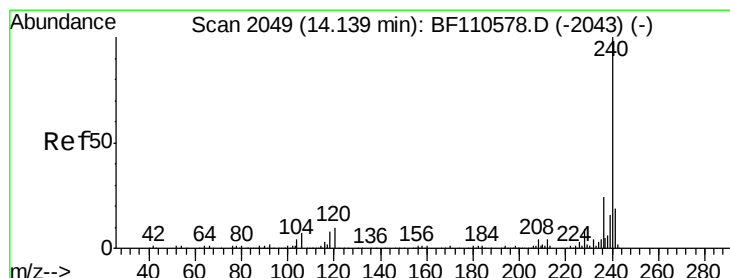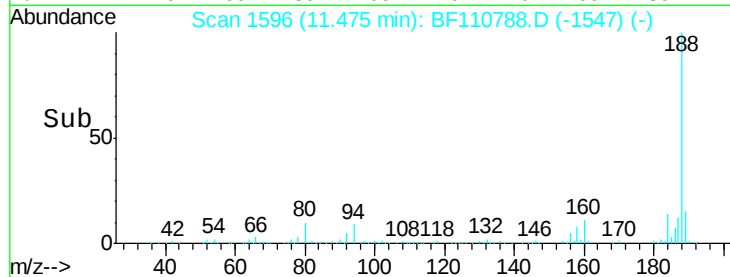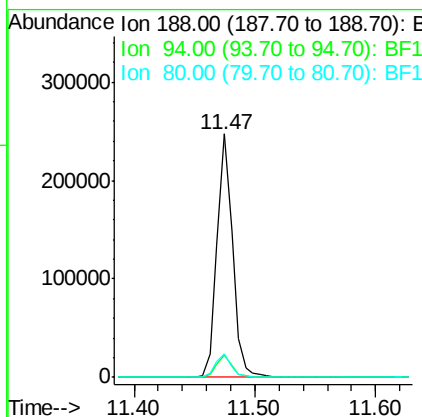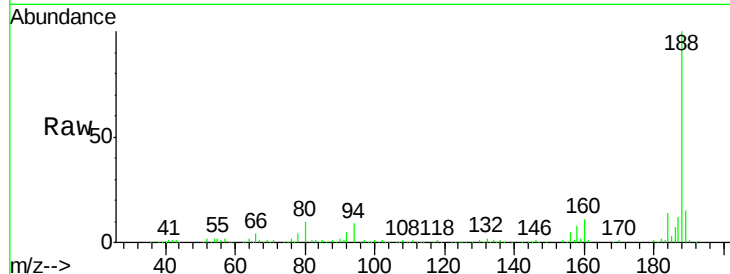

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110788.D
Acq: 15 Nov 2018 15:11

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	148277		
120	10.9		8.3	12.5
236	25.1		21.2	31.8

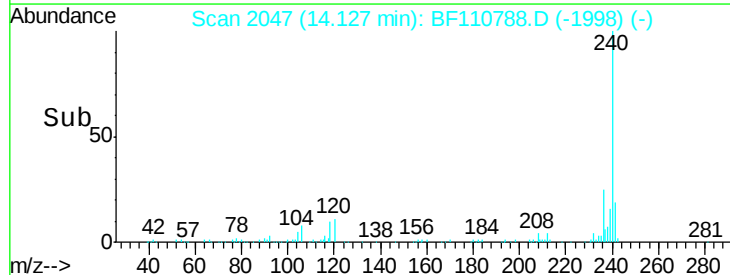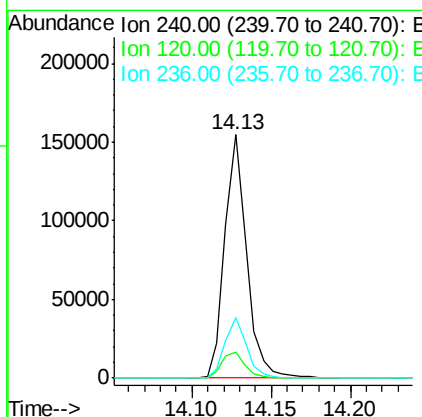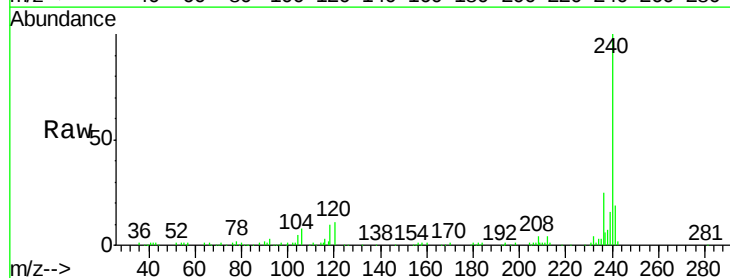

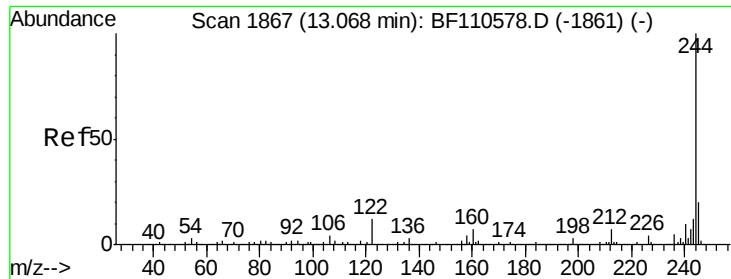

#79

Terphenyl-d14

Concen: 50.768 ng

RT: 13.06 min Scan# 1865

Delta R.T. -0.01 min

Lab File: BF110788.D

Acq: 15 Nov 2018 15:11

Instrument :

BNA_F

ClientSampleId :

SSI-21-TW-2


Tgt Ion:244 Resp: 401957

Ion Ratio Lower Upper

244 100

212 6.5 5.8 8.8




122 11.2 8.7 13.1

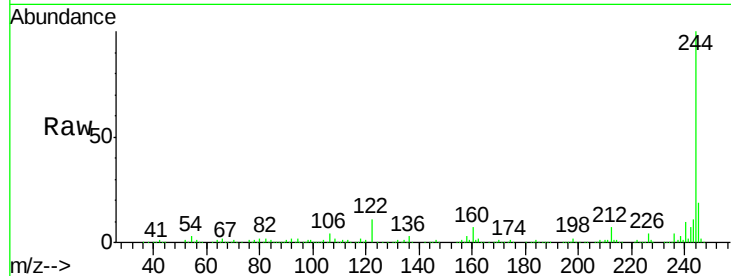

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

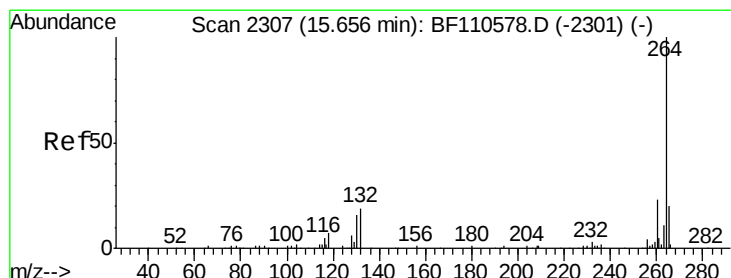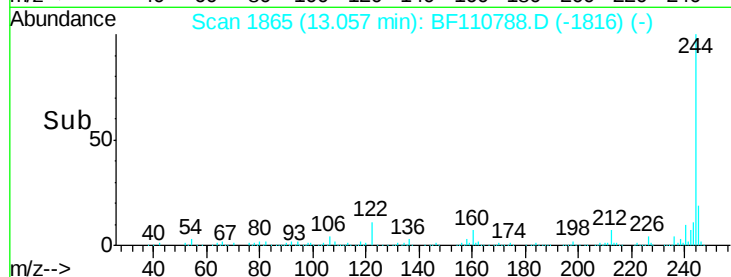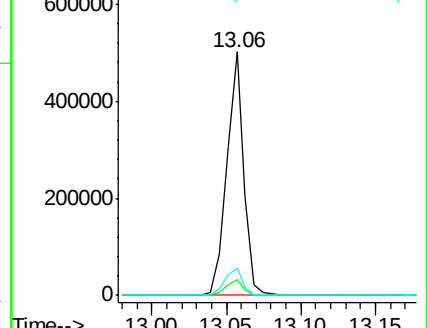

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.66 min Scan# 2307

Delta R.T. 0.00 min

Lab File: BF110788.D

Acq: 15 Nov 2018 15:11


Tgt Ion:264 Resp: 139250

Ion Ratio Lower Upper

264 100

260 21.4 18.7 28.1

265 21.1 16.7 25.1

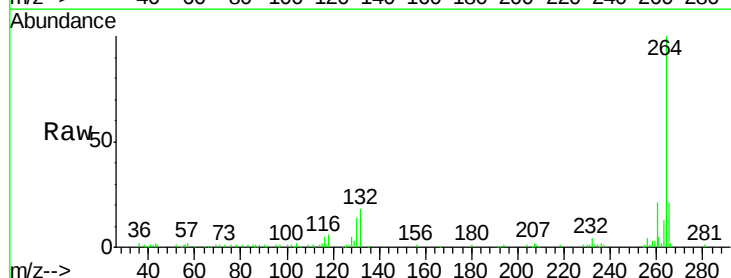

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

