


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111518\
 Data File : BF110783.D
 Acq On : 15 Nov 2018 11:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 12:43:10 2018

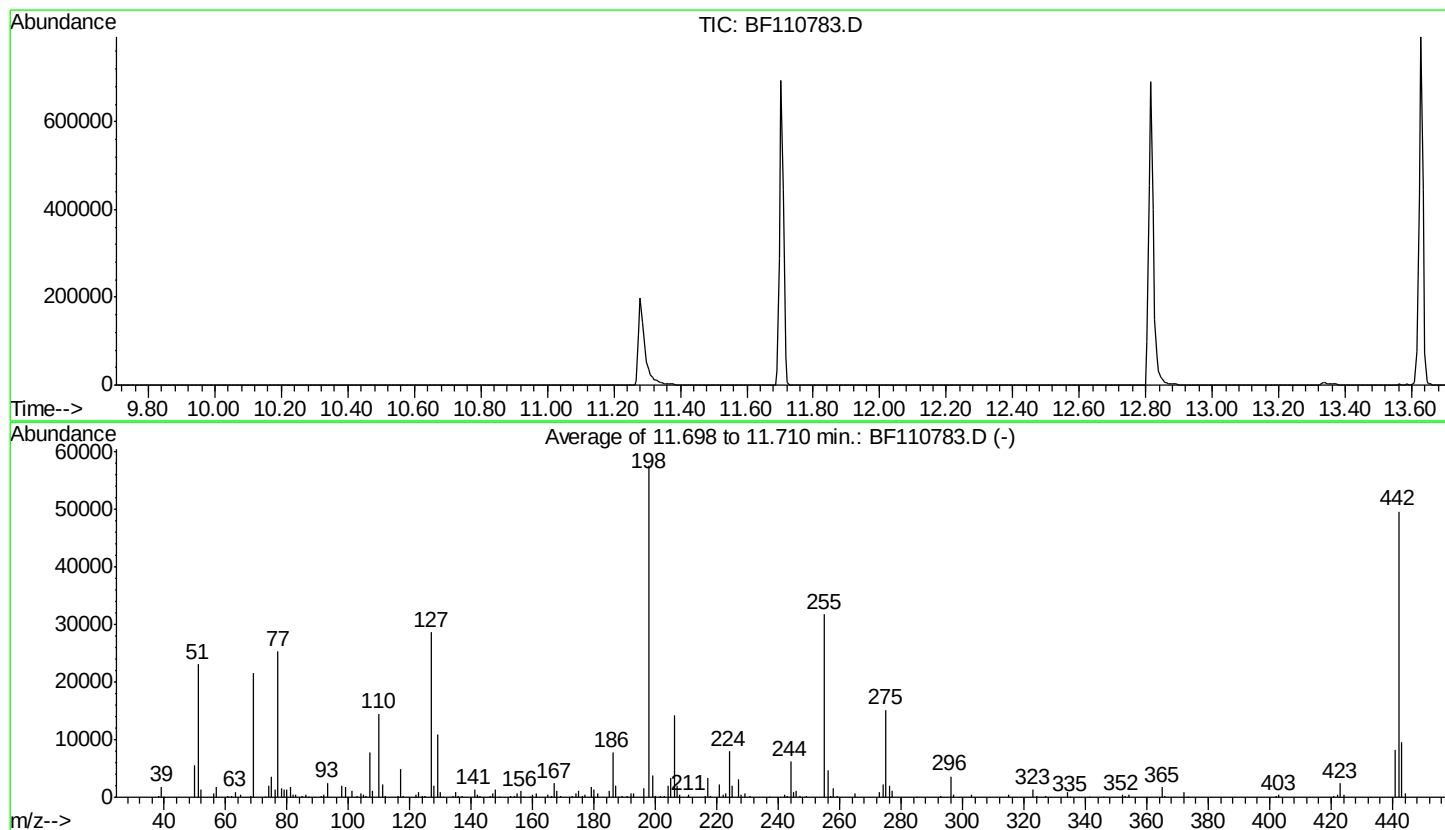

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	23022	PASS
68	69	0.00	2	1.0	207	PASS
69	198	0.00	100	37.6	21630	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	28584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57557	PASS
199	198	5	9	6.5	3732	PASS
275	198	10	60	26.3	15138	PASS
365	198	1	100	3.0	1719	PASS
441	198	0.01	100	14.3	8237	PASS
442	198	50	100	86.3	49661	PASS
443	442	15	24	19.1	9501	PASS