
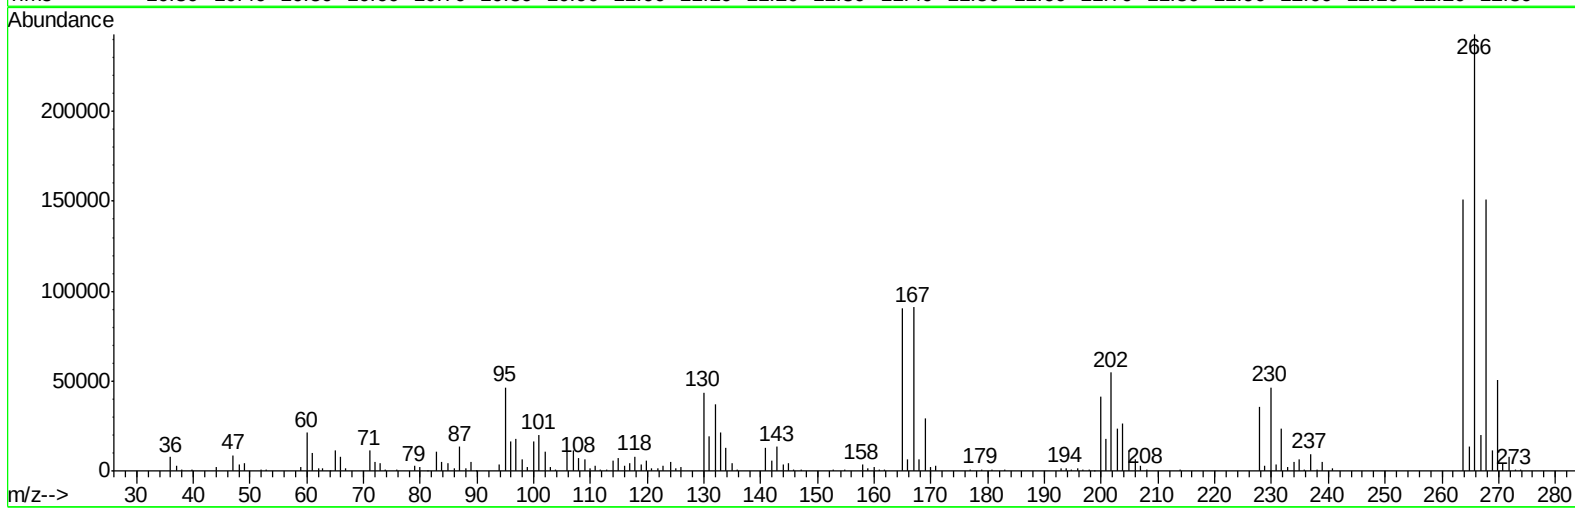


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111519\
Data File : BF117801.D
Acq On : 15 Nov 2019 14:22
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 04:31:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

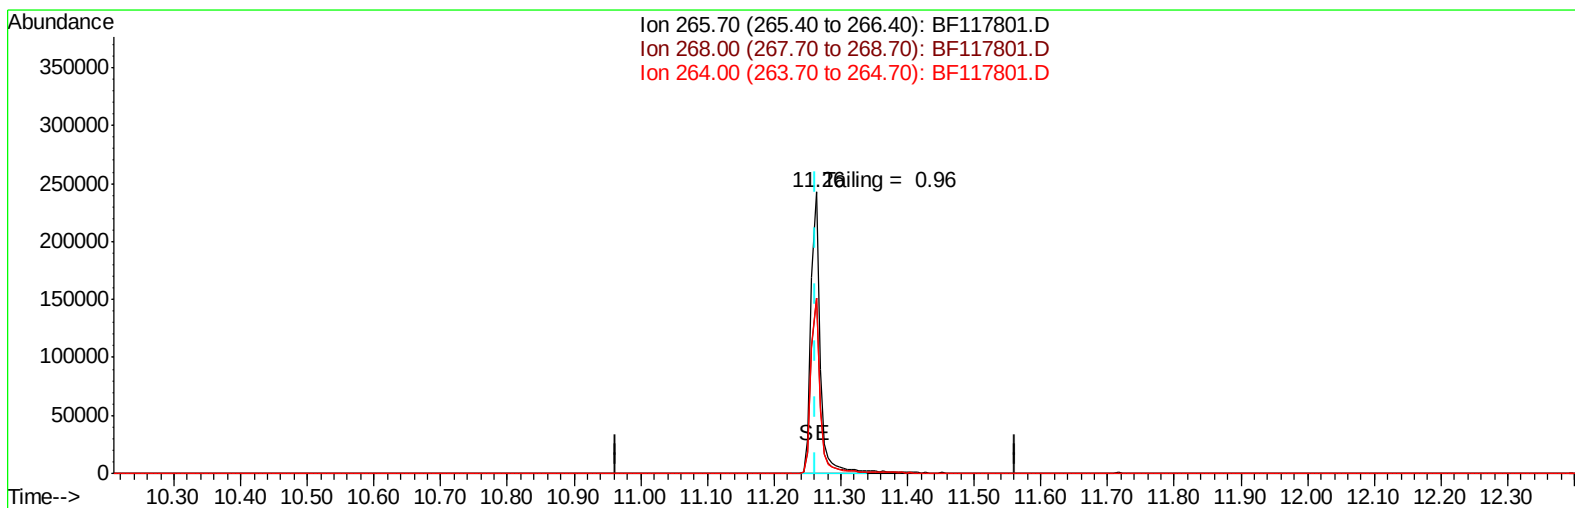

TIC: BF117801.D

(70) Pentachlorophenol (C)

11.263min (-0.000) 46457.21ng

response 221282

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	62.13
264.00	63.40	62.24
0.00	0.00	0.00

