

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111519\
 Data File : BF117821.D
 Acq On : 15 Nov 2019 23:35
 Operator : JU
 Sample : K5861-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EP-5

Quant Time: Nov 18 03:32:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 18:36:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.92	152	261305	20.00	ng	0.00
21) Naphthalene-d8	8.20	136	1032646	20.00	ng	-0.01
39) Acenaphthene-d10	9.97	164	547358	20.00	ng	0.00
64) Phenanthrene-d10	11.46	188	1045985	20.00	ng	-0.01
76) Chrysene-d12	14.10	240	773475	20.00	ng	-0.01
87) Perylene-d12	15.62	264	796438	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	1541944	104.45	ng	0.00
7) Phenol-d6	6.54	99	1914708	107.53	ng	0.00
23) Nitrobenzene-d5	7.48	82	1176407	67.72	ng	-0.01
42) 2,4,6-Tribromophenol	10.76	330	591083	102.00	ng	-0.01
45) 2-Fluorobiphenyl	9.29	172	2214800	72.59	ng	0.00
79) Terphenyl-d14	13.05	244	2642987	62.45	ng	0.00
Target Compounds						
10) Phenol	6.55	94	49152	2.657	ng	93
50) Dimethylphthalate	9.67	163	250205	6.519	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111519\
Data File : BF117821.D
Acq On : 15 Nov 2019 23:35
Operator : JU
Sample : K5861-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EP-5

Quant Time: Nov 18 03:32:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

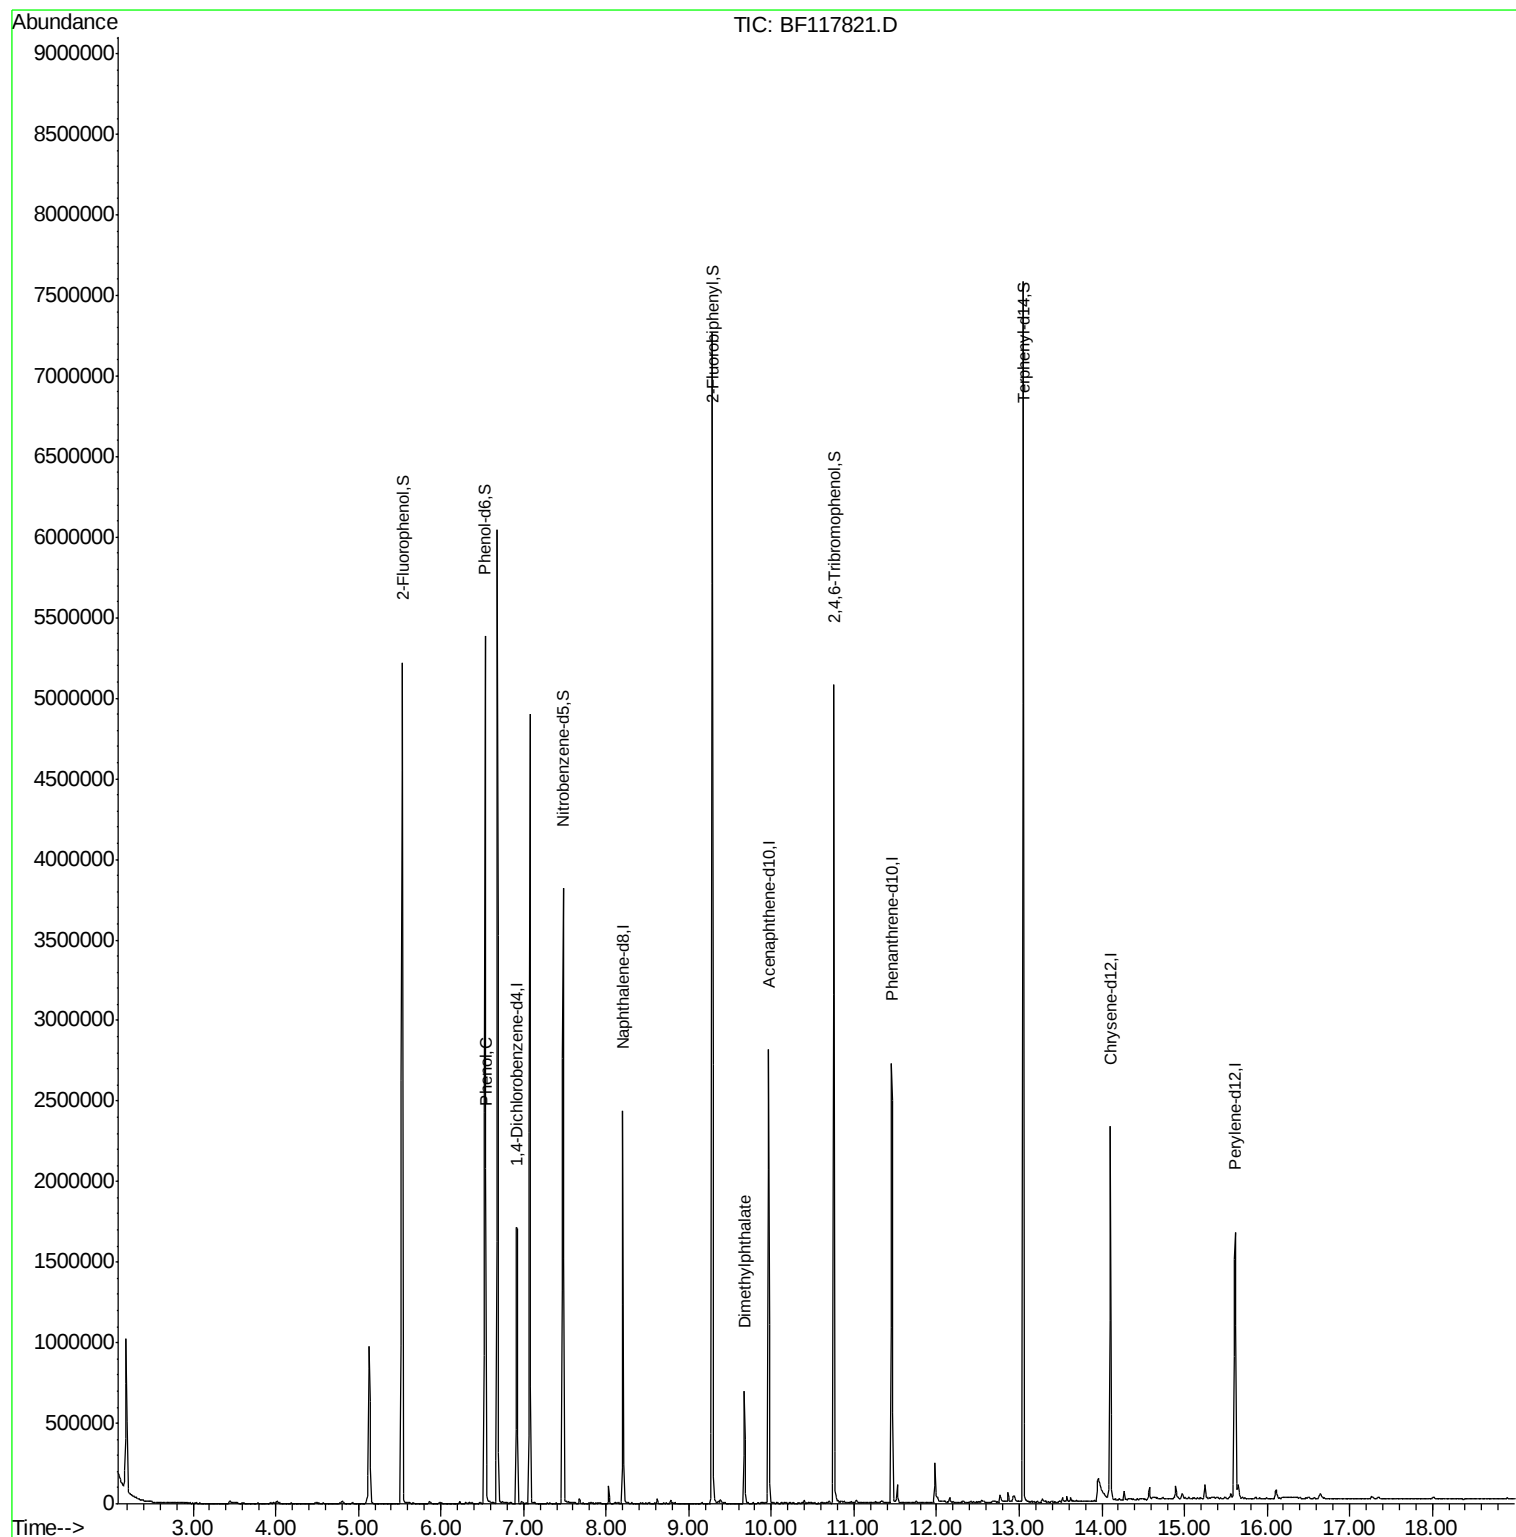

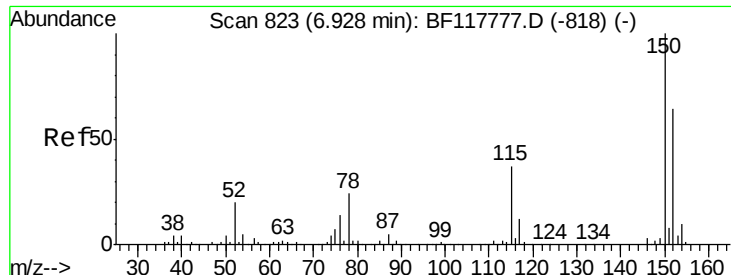


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.92 min Scan# 822
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Instrument :
BNA_F
ClientSampleId :
EP-5

Tot Ion:152 Resp: 261305
Ion Ratio Lower Upper
152 100
150 157.4 125.3 187.9
115 58.3 47.0 70.4

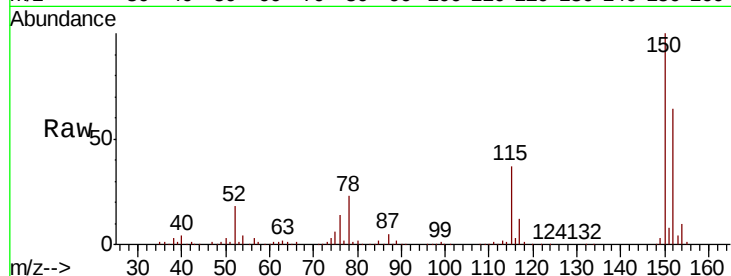


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

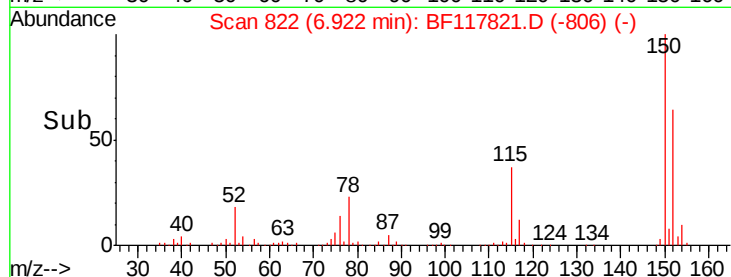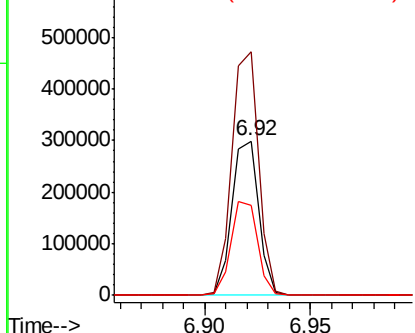



#5


2-Fluorophenol
Concen: 104.453 ng
RT: 5.53 min Scan# 586
Delta R.T. -0.00 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Tgt Ion:112 Resp: 1541944
Ion Ratio Lower Upper
112 100
64 55.2 45.6 68.4
63 29.4 24.1 36.1

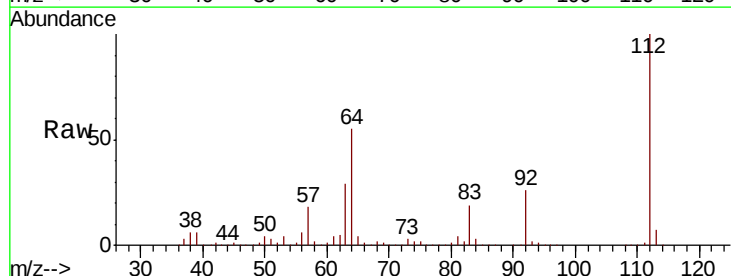

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

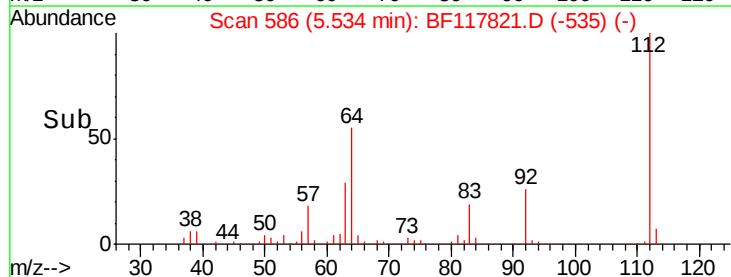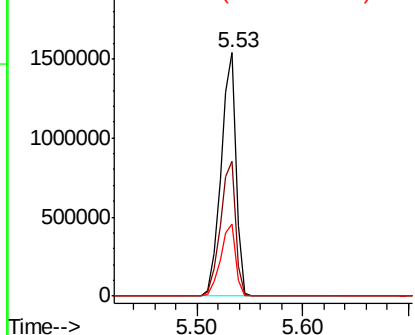

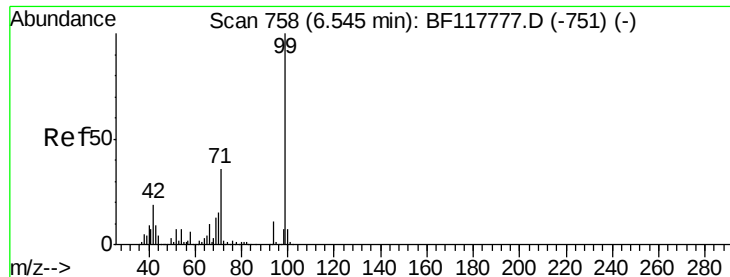

#7

Phenol-d6

Concen: 107.535 ng

RT: 6.54 min Scan# 757

Delta R.T. -0.01 min

Lab File: BF117821.D

Acq: 15 Nov 2019 23:35

Instrument :

BNA_F

ClientSampleId :

EP-5


Tot Ion: 99 Resp: 1914708

Ion Ratio Lower Upper




99 100

42 18.7 14.9 22.3

71 36.4 28.6 43.0

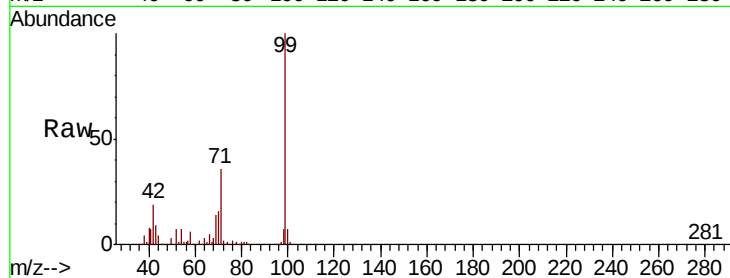

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

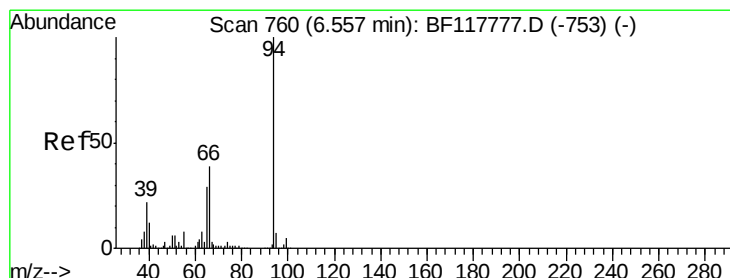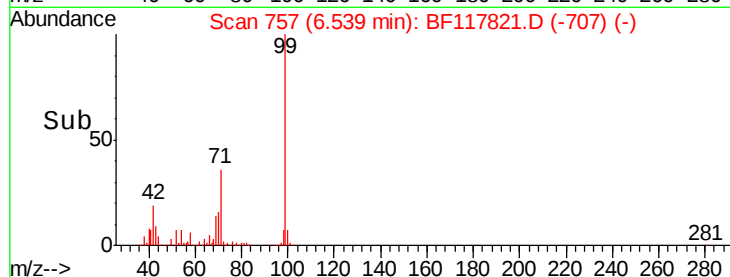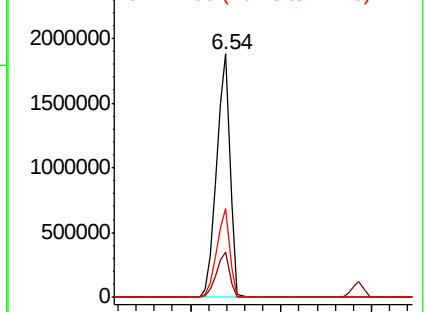

#10

Phenol

Concen: 2.657 ng

RT: 6.55 min Scan# 759

Delta R.T. -0.01 min

Lab File: BF117821.D

Acq: 15 Nov 2019 23:35


Tgt Ion: 94 Resp: 49152

Ion Ratio Lower Upper



94 100

65 25.4 8.9 48.9

66 34.3 18.7 58.7

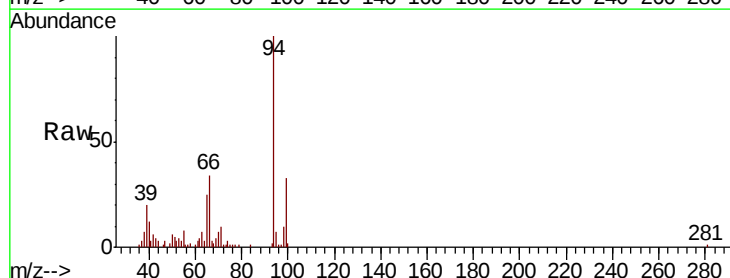

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

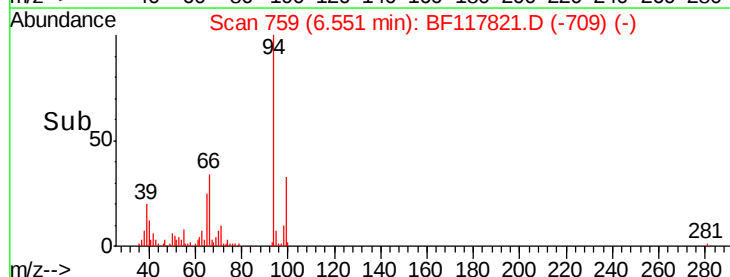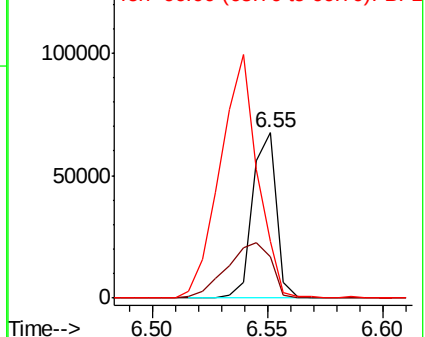







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.20 min Scan# 1040
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Instrument :
BNA_F
ClientSampleId :
EP-5

Tot Ion:136 Resp: 1032646
Ion Ratio Lower Upper
136 100
137 11.1 9.0 13.4
54 7.6 5.4 8.2
68 5.8 4.3 6.5

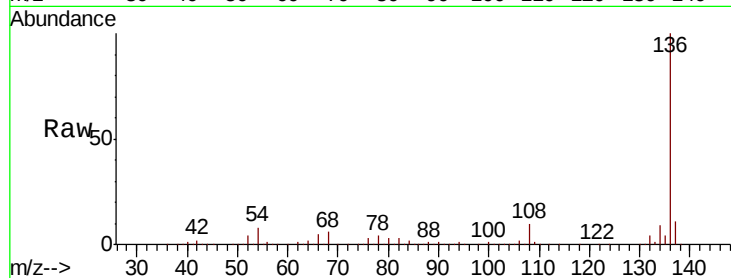


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

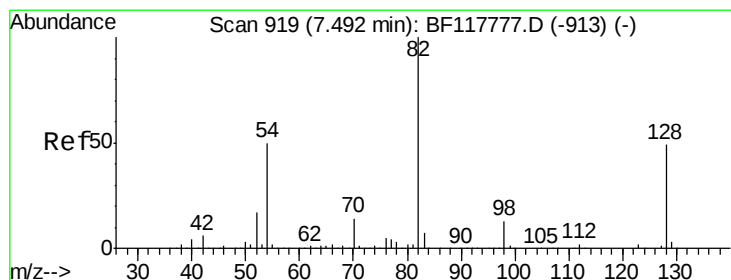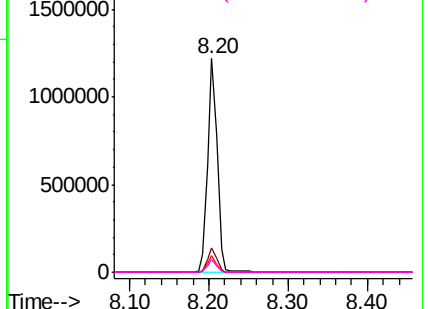
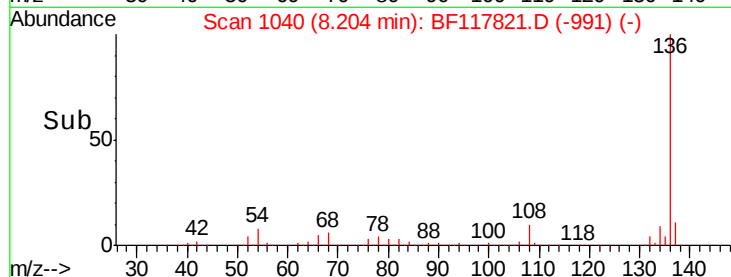



#23
Nitrobenzene-d5
Concen: 67.722 ng
RT: 7.48 min Scan# 917
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Tgt Ion: 82 Resp: 1176407
Ion Ratio Lower Upper
82 100
128 49.2 38.9 58.3
54 50.5 39.8 59.6

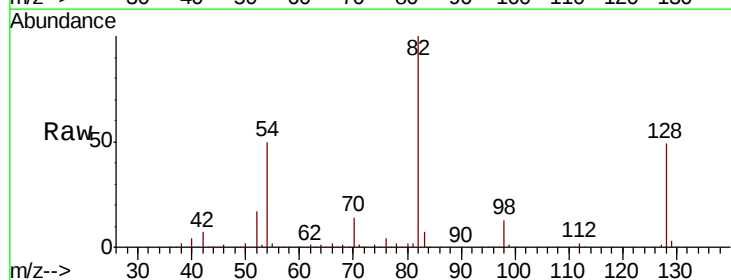

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

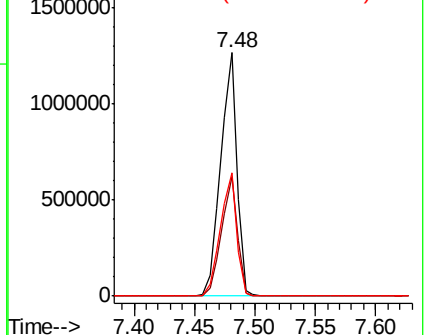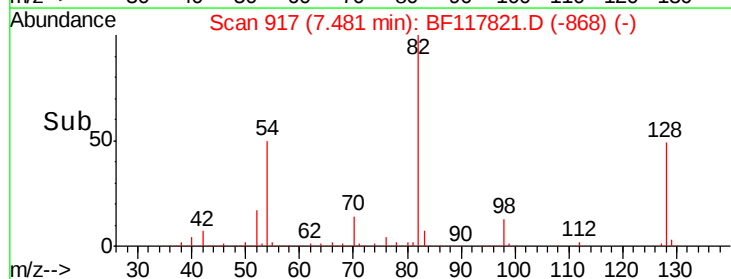


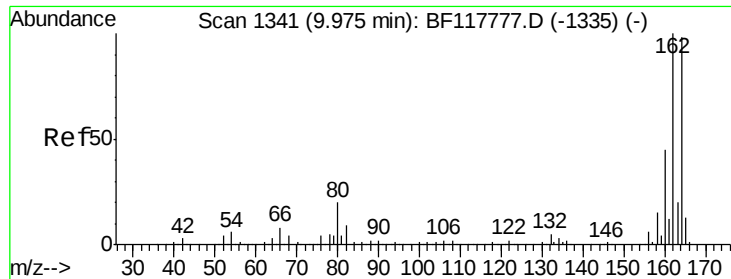




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.97 min Scan# 1340
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Instrument :
BNA_F
ClientSampleId :
EP-5

Tot Ion:164 Resp: 547358
Ion Ratio Lower Upper
164 100
162 100.4 81.3 121.9
160 44.8 36.6 55.0

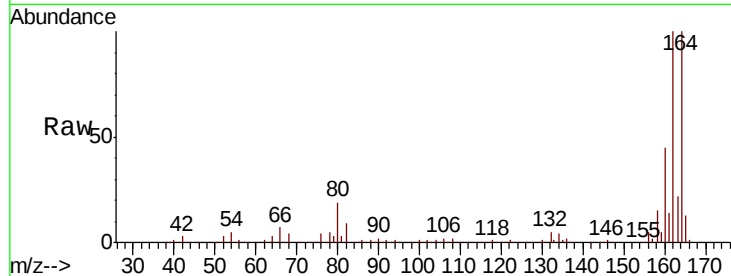


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

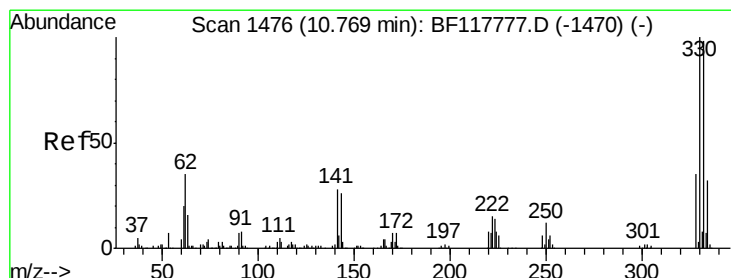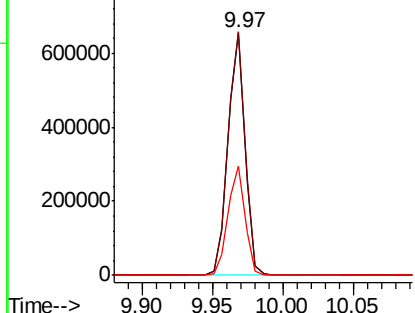
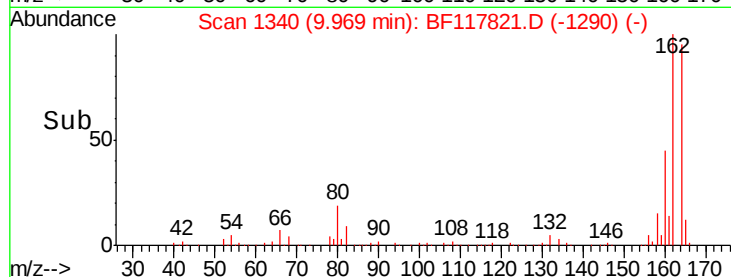



#42
2,4,6-Tribromophenol
Concen: 102.002 ng
RT: 10.76 min Scan# 1474
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Tgt Ion:330 Resp: 591083
Ion Ratio Lower Upper
330 100
332 95.8 76.7 115.1
141 33.4 27.7 41.5

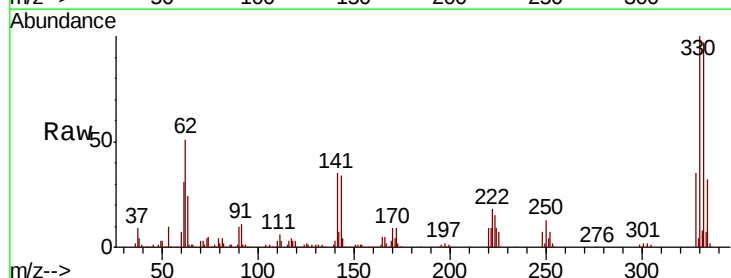

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

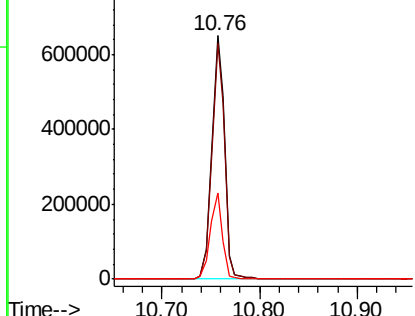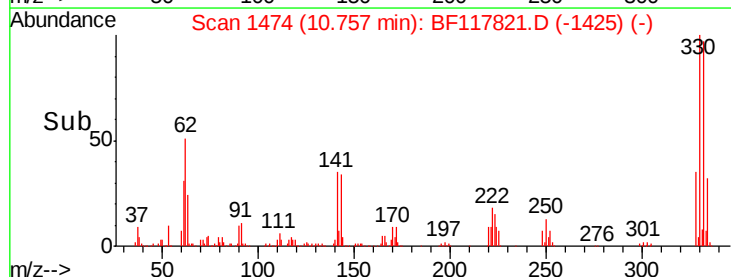


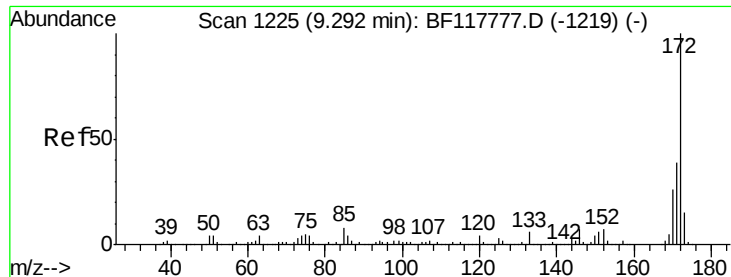




#45
2-Fluorobiphenyl
Concen: 72.593 ng
RT: 9.29 min Scan# 1224
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Instrument :
BNA_F
ClientSampleId :
EP-5

Tot Ion:172 Resp: 2214800
Ion Ratio Lower Upper
172 100
171 37.5 30.9 46.3
170 24.7 21.0 31.4

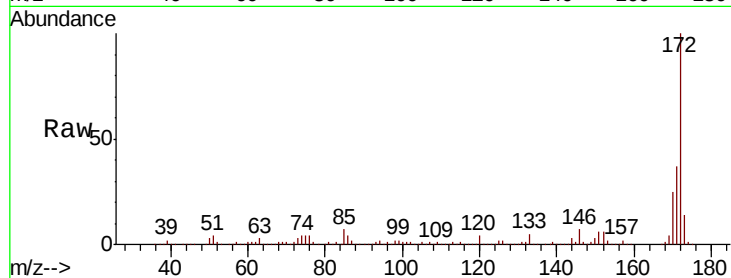


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

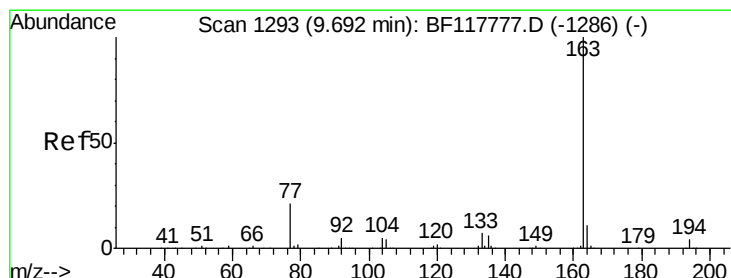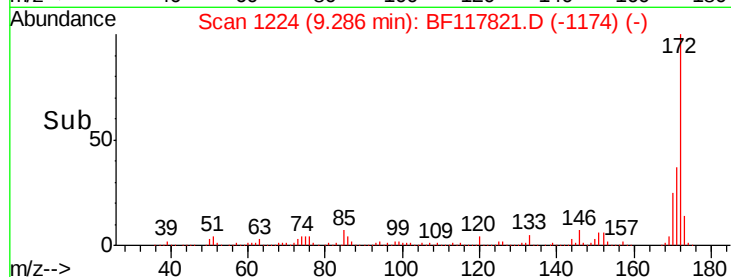
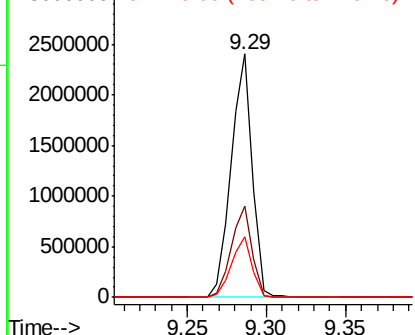



#50
Dimethylphthalate
Concen: 6.519 ng
RT: 9.67 min Scan# 1290
Delta R.T. -0.02 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Tgt Ion:163 Resp: 250205
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.2 8.7 13.1

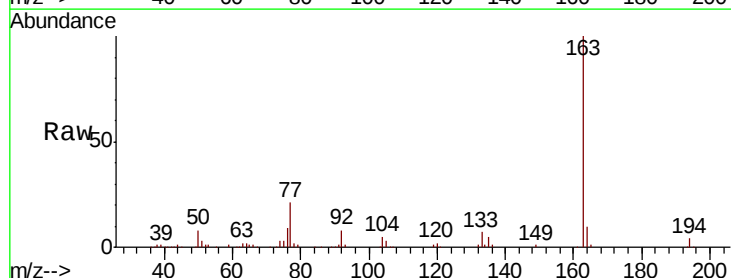

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

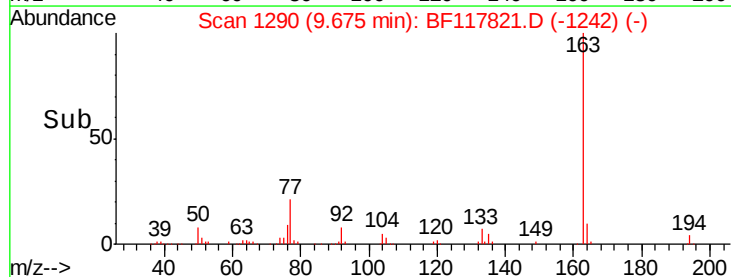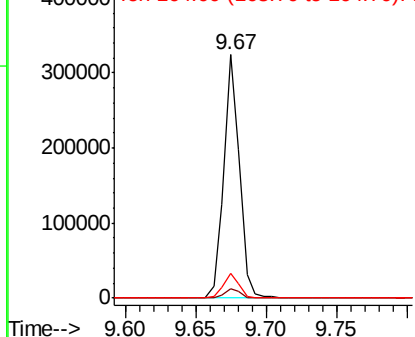


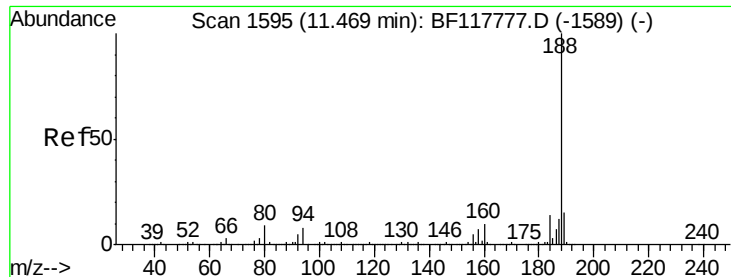




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.46 min Scan# 1593
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Instrument :
BNA_F
ClientSampleId :
EP-5

Tot Ion:188 Resp: 1045985
Ion Ratio Lower Upper
188 100
94 9.8 6.6 10.0
80 11.1 7.2 10.8#

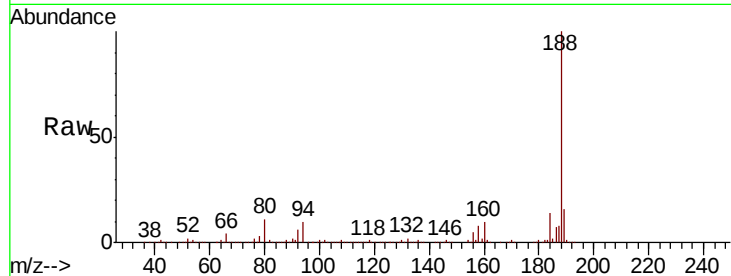


Abundance Ion 188.00 (187.70 to 188.70): E
1500000 Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

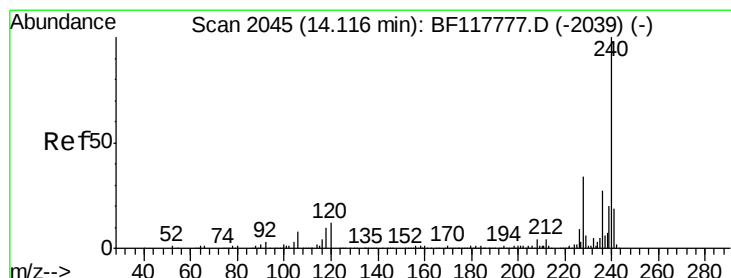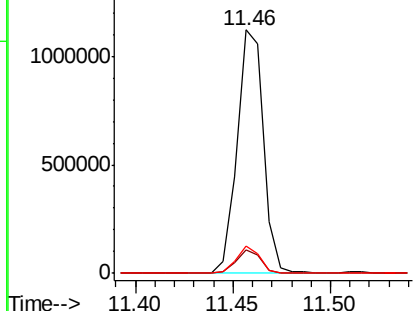
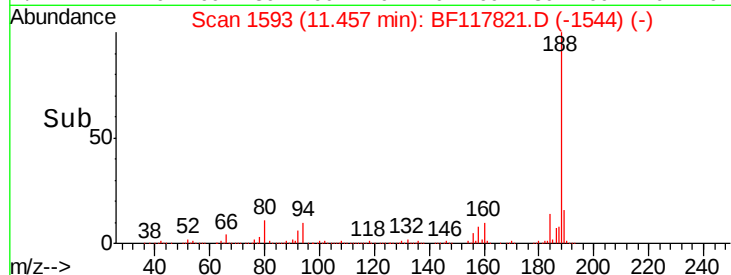



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.10 min Scan# 2043
Delta R.T. -0.01 min
Lab File: BF117821.D
Acq: 15 Nov 2019 23:35

Tgt Ion:240 Resp: 773475
Ion Ratio Lower Upper
240 100
120 12.2 9.5 14.3
236 25.9 21.3 31.9

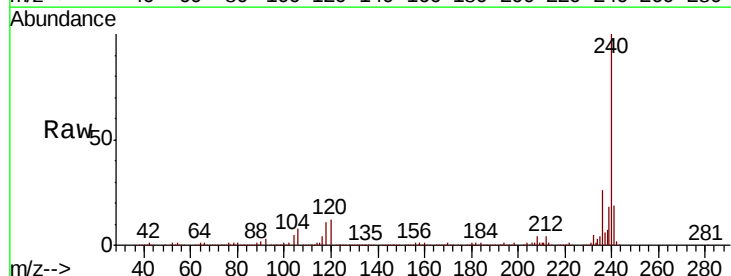

Abundance Ion 240.00 (239.70 to 240.70): E
1000000 Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

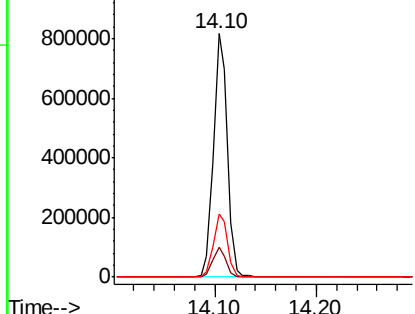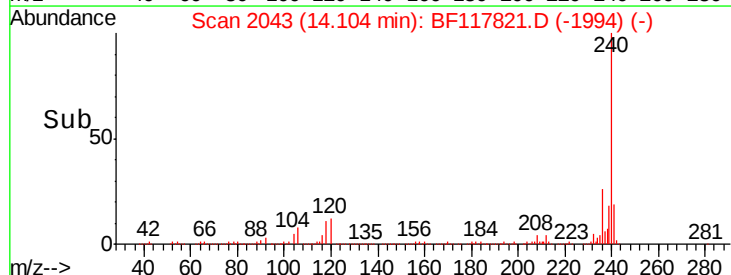

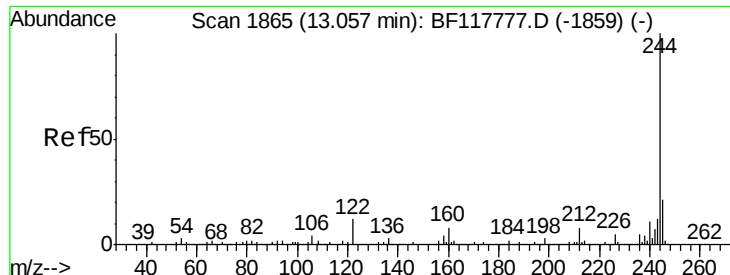

#79

Terphenyl-d14

Concen: 62.450 ng

RT: 13.05 min Scan# 1864

Delta R.T. -0.01 min

Lab File: BF117821.D

Acq: 15 Nov 2019 23:35

Instrument :


BNA_F

ClientSampleId :

EP-5

Tot Ion:244 Resp: 2642987




Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.3	9.5
122	11.8	9.4	14.2

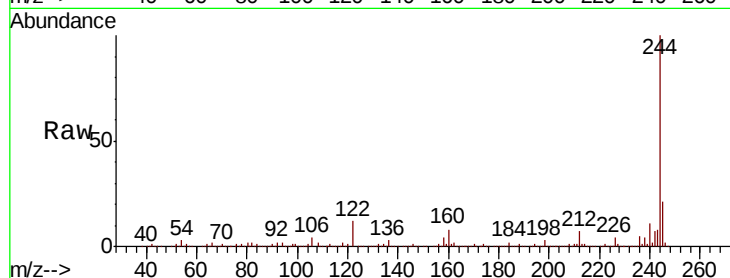

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

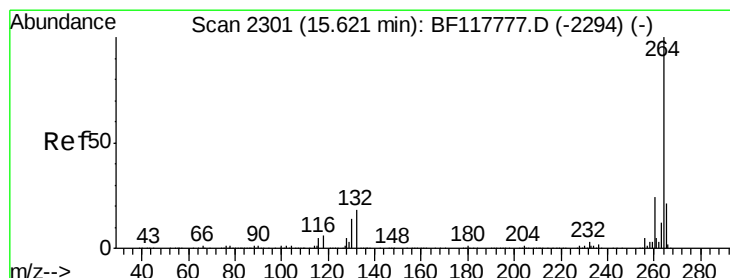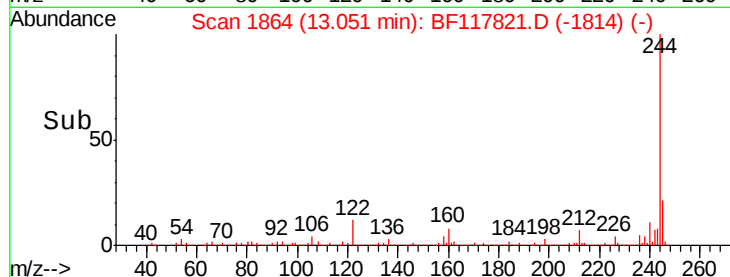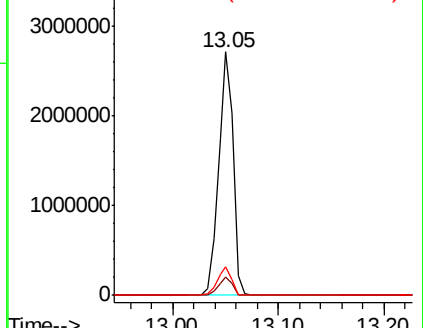

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.62 min Scan# 2300


Delta R.T. -0.01 min

Lab File: BF117821.D

Acq: 15 Nov 2019 23:35

Tgt Ion:264 Resp: 796438

Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.4	29.0
265	22.4	17.1	25.7

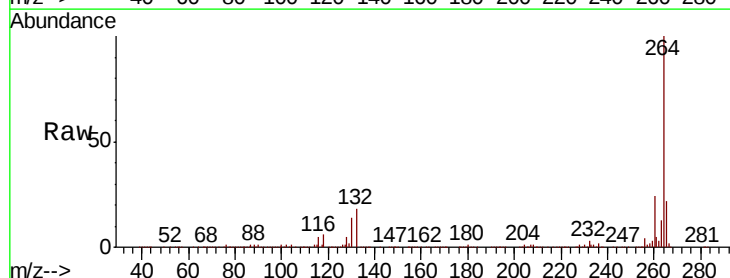

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

