


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111519\
 Data File : BF117794.D
 Acq On : 15 Nov 2019 9:01
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

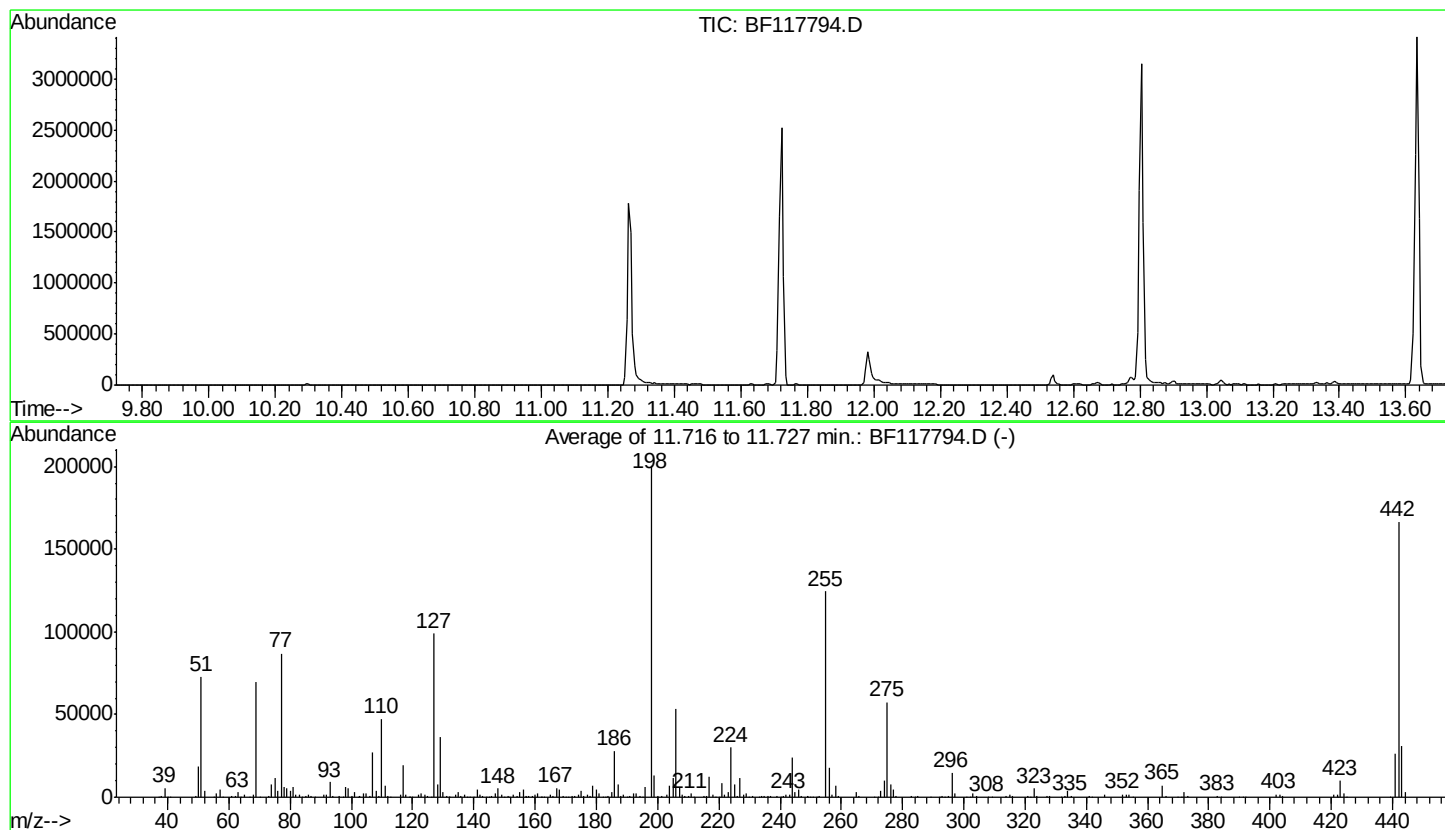

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	73093	PASS
68	69	0.00	2	1.8	1240	PASS
69	198	0.00	100	34.9	69946	PASS
70	69	0.00	2	0.4	306	PASS
127	198	10	80	49.2	98749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	200514	PASS
199	198	5	9	6.7	13382	PASS
275	198	10	60	28.8	57664	PASS
365	198	1	100	3.7	7344	PASS
441	198	0.01	100	13.3	26733	PASS
442	198	50	100	83.2	166813	PASS
443	442	15	24	18.5	30909	PASS