


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111519\
 Data File : BF117801.D
 Acq On : 15 Nov 2019 14:22
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

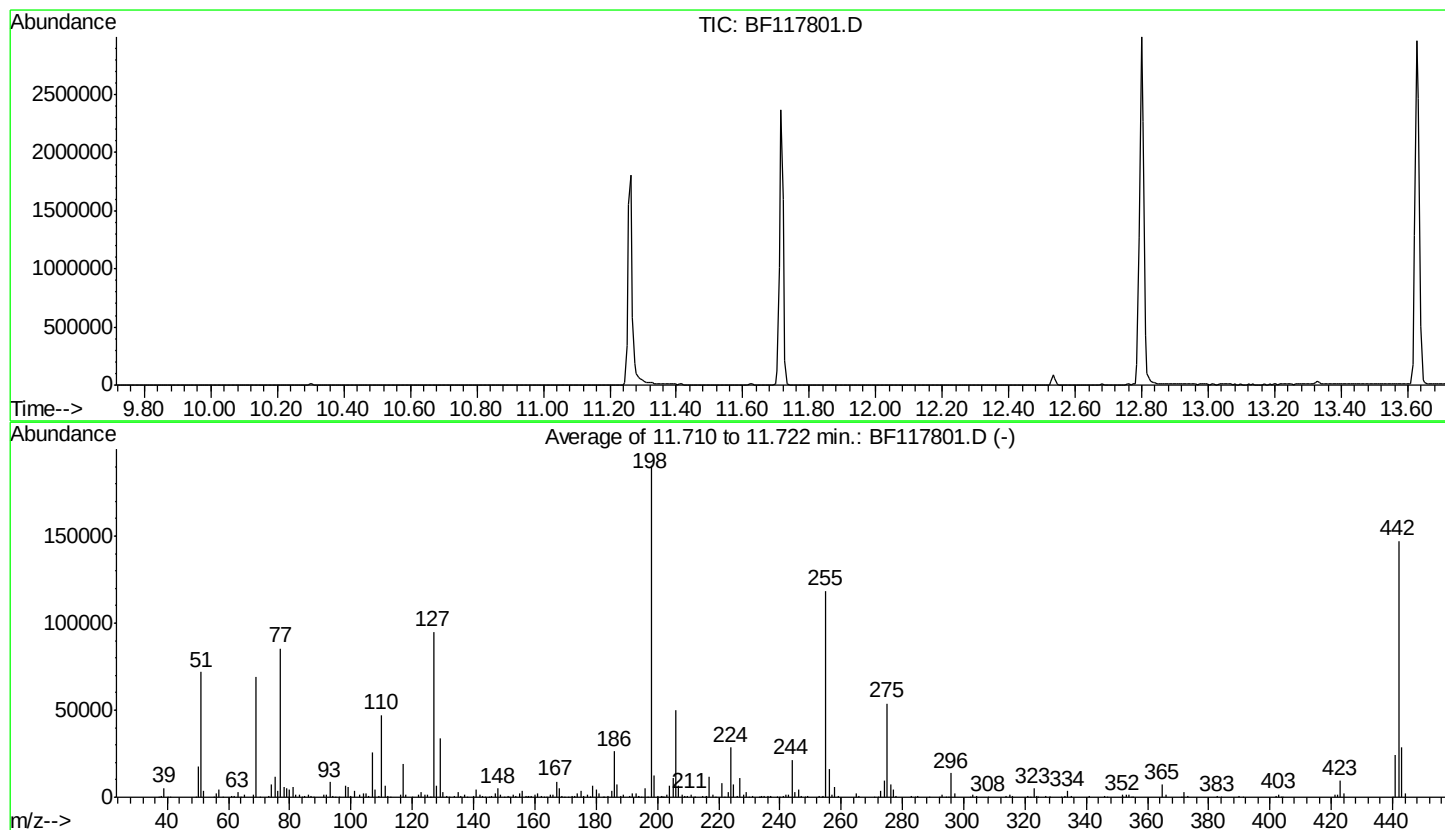

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	71925	PASS
68	69	0.00	2	1.9	1319	PASS
69	198	0.00	100	36.4	69237	PASS
70	69	0.00	2	0.5	330	PASS
127	198	10	80	49.9	94997	PASS
197	198	0.00	2	0.1	282	PASS
198	198	100	100	100.0	190386	PASS
199	198	5	9	6.5	12433	PASS
275	198	10	60	28.3	53904	PASS
365	198	1	100	3.7	7040	PASS
441	198	0.01	100	12.7	24135	PASS
442	198	50	100	77.3	147208	PASS
443	442	15	24	19.5	28638	PASS