
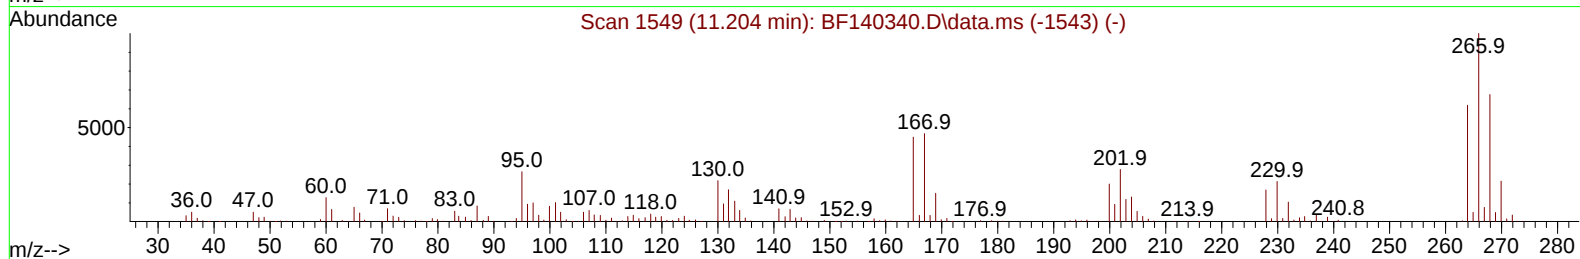
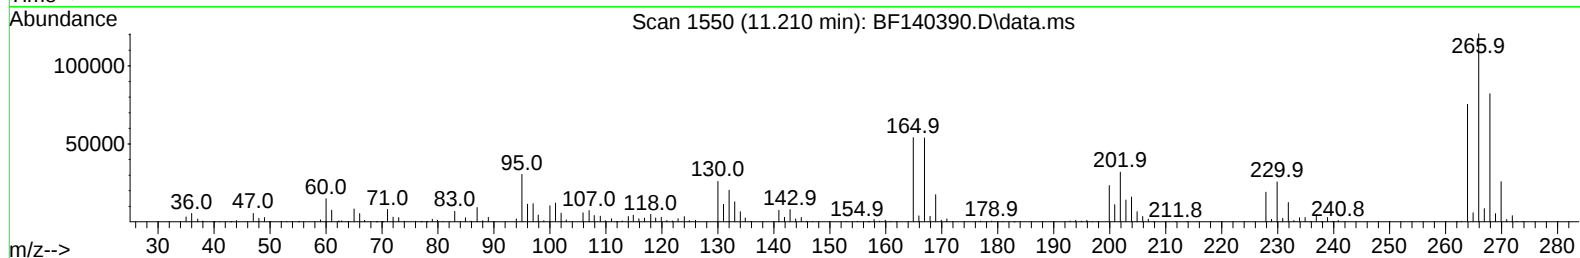


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111524\
Data File : BF140390.D
Acq On : 15 Nov 2024 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 10:40:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

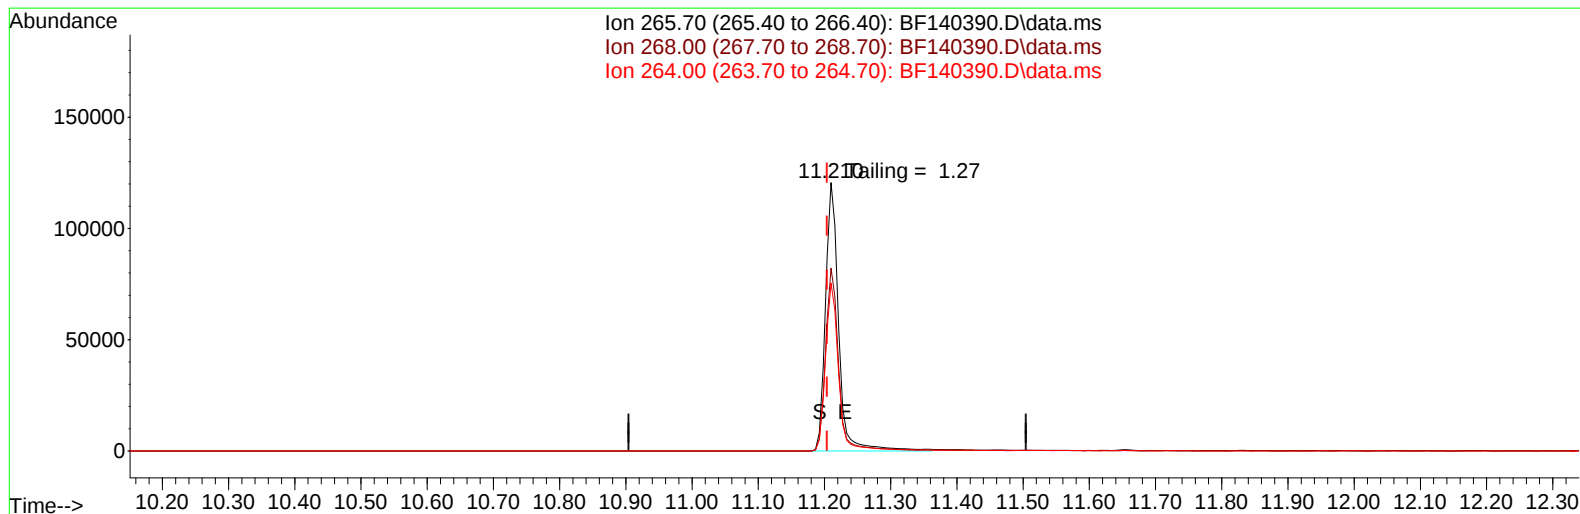

TIC: BF140390.D\data.ms

(70) Pentachlorophenol (C)




11.210min (+ 0.006) 50509.13 ng

response 166467

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	68.10
264.00	62.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111524\
Data File : BF140390.D
Acq On : 15 Nov 2024 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 10:40:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

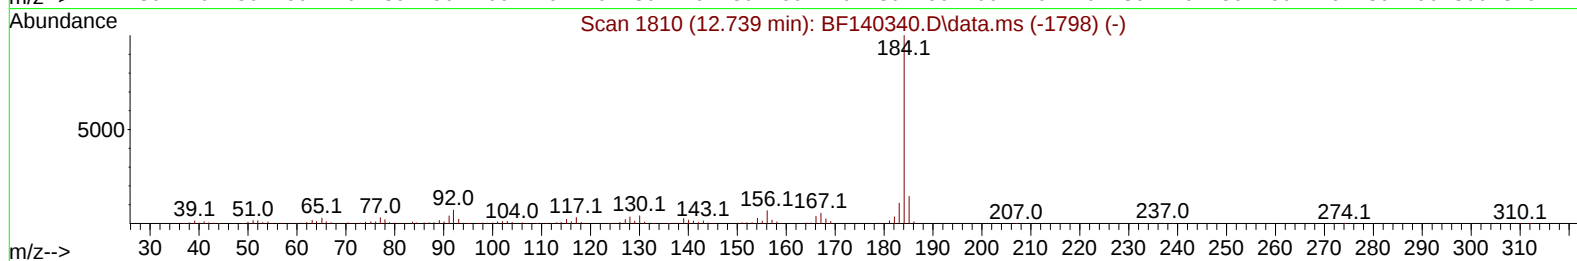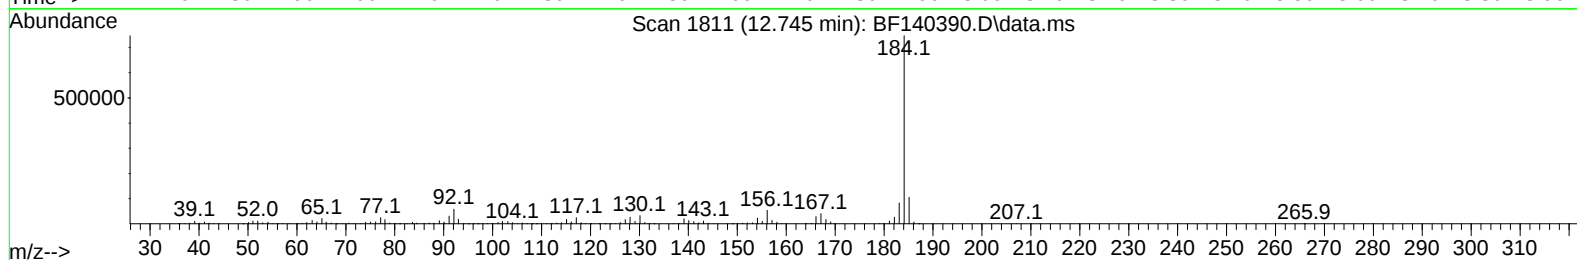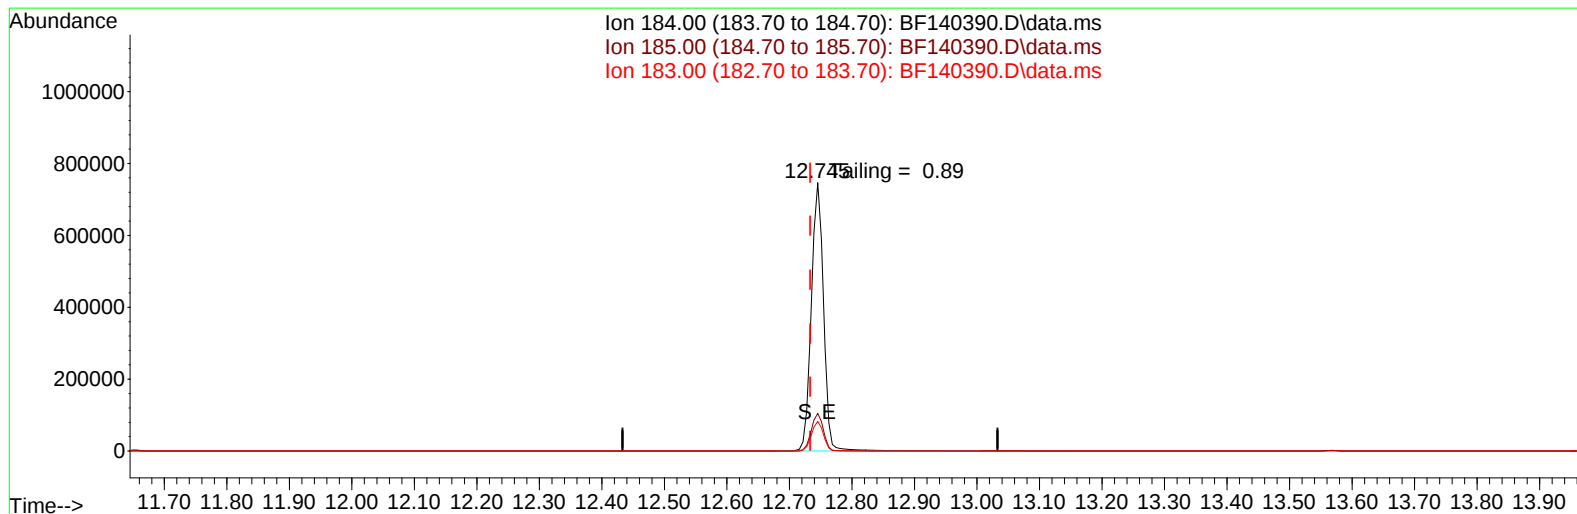

TIC: BF140390.D\data.ms

(77) Benzidine

12.745min (+ 0.012) 31749.52 ng

response 1013847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.05
183.00	10.80	11.05
0.00	0.00	0.00