
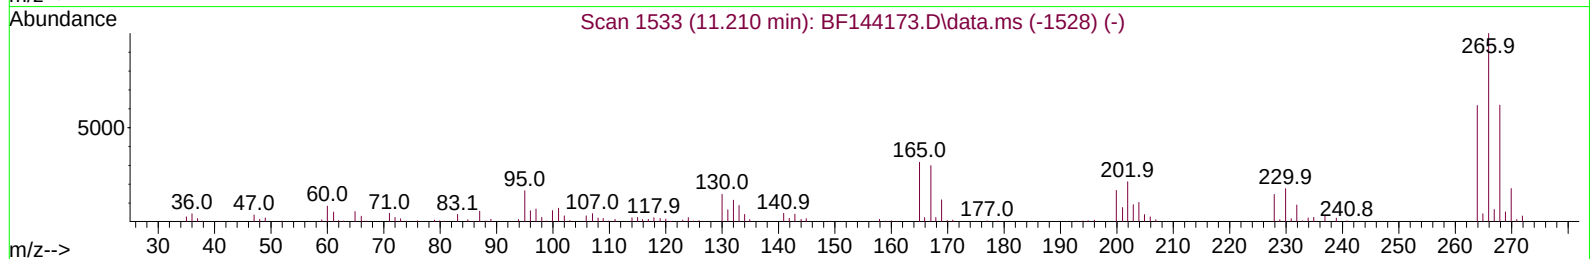
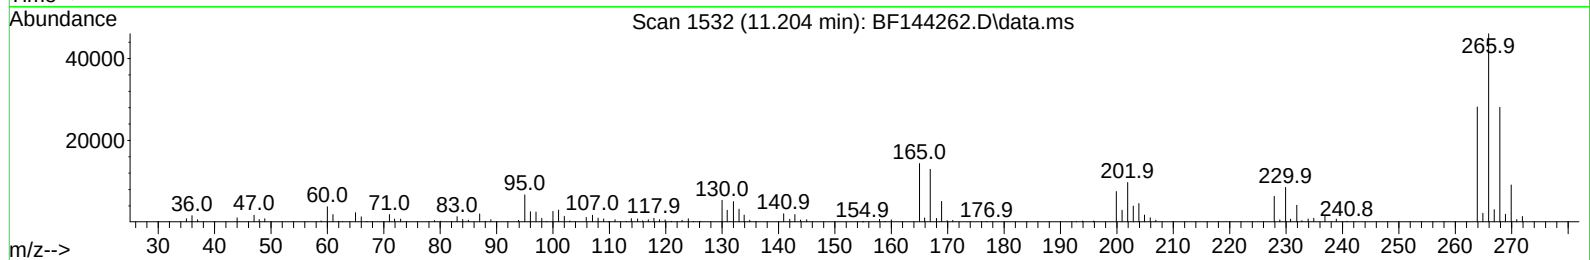


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111725\
Data File : BF144262.D
Acq On : 17 Nov 2025 12:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 12:57:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

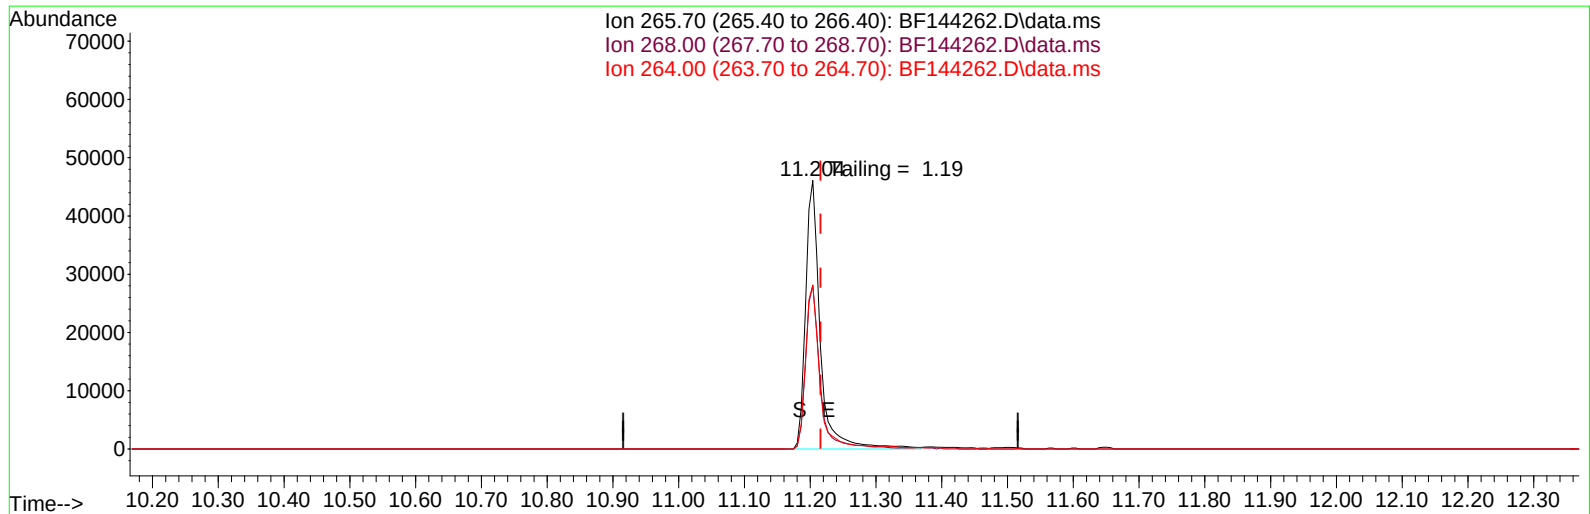

TIC: BF144262.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.012) 32389.41 ng

response 72018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	60.95
264.00	61.80	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111725\
Data File : BF144262.D
Acq On : 17 Nov 2025 12:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 12:57:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

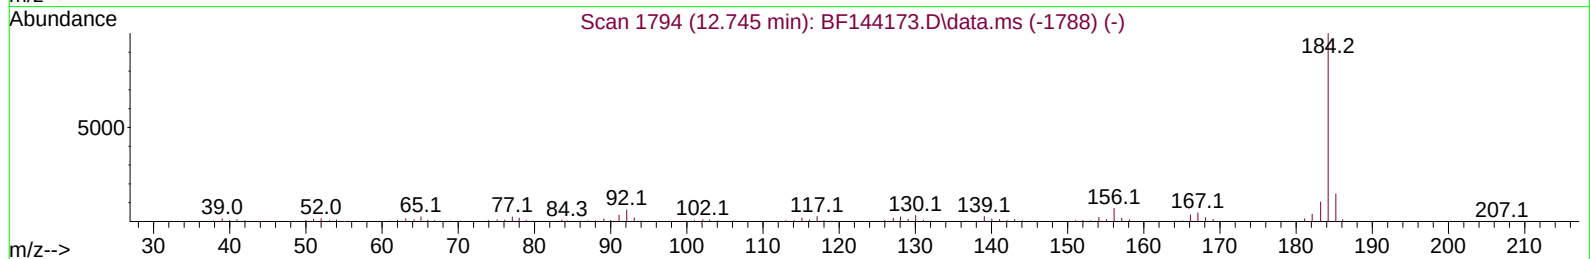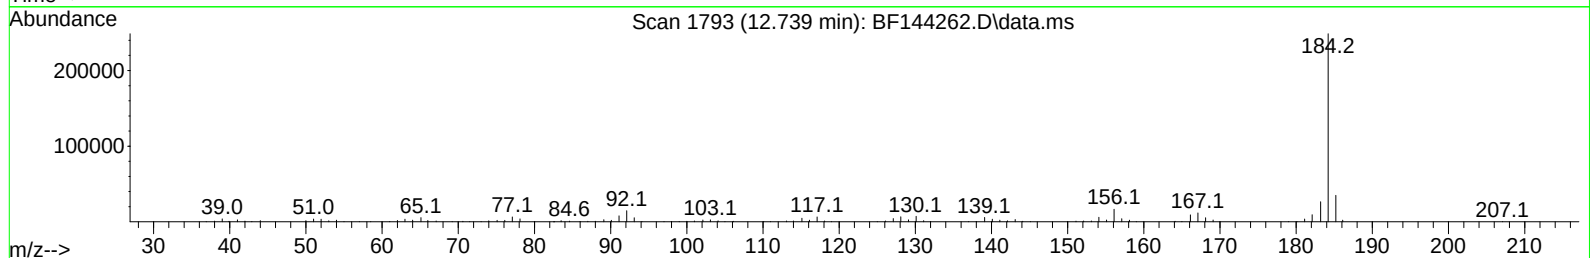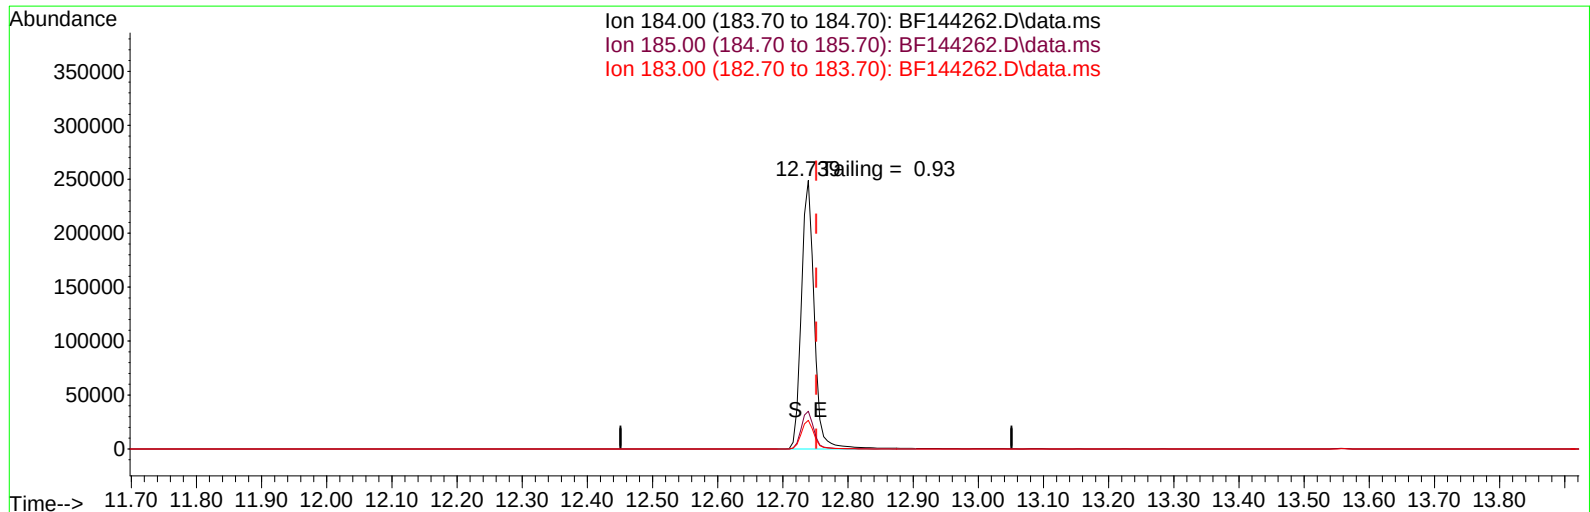

TIC: BF144262.D\data.ms

(77) Benzidine

12.739min (-0.012) 0.00 ng

response 342050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.06
183.00	10.40	10.65
0.00	0.00	0.00