
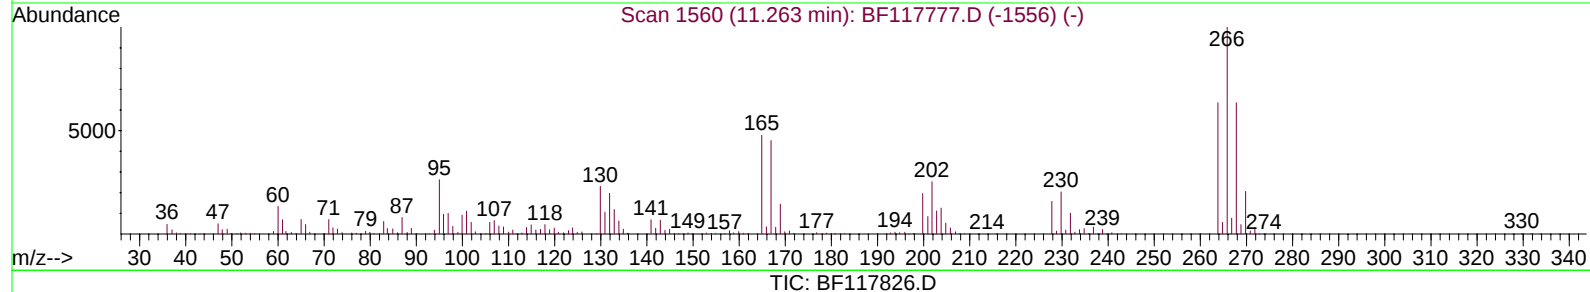
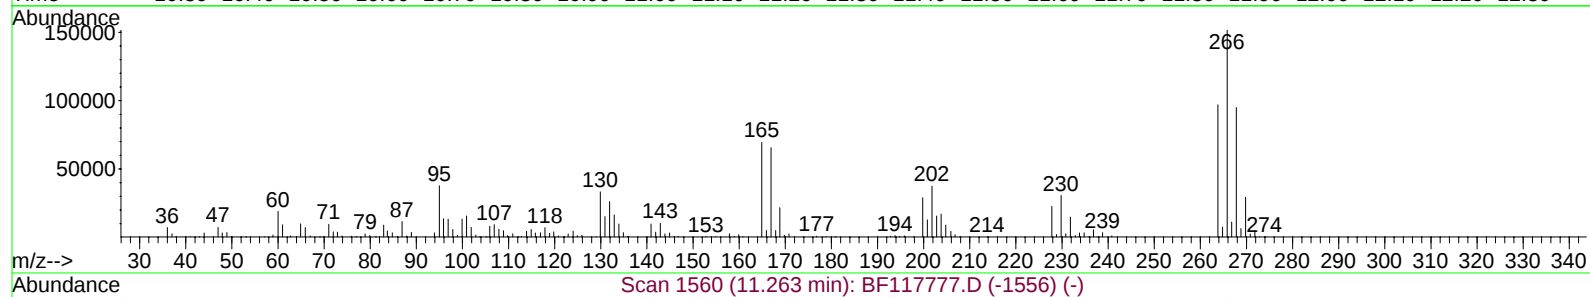


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111819\
 Data File : BF117826.D
 Acq On : 18 Nov 2019 10:57
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 17:57:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 18:36:07 2019
 Response via : Initial Calibration

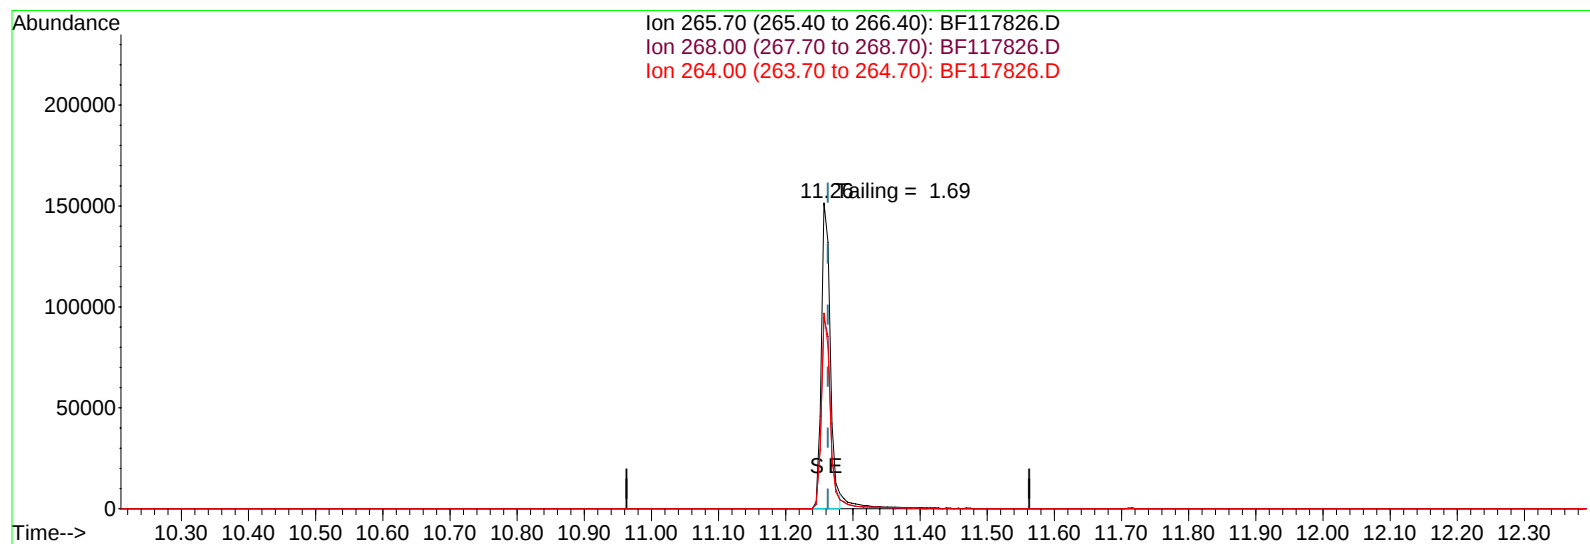

(70) Pentachlorophenol (C)




11.257min (-0.006) 91951.52ng

response 149372

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	62.67
264.00	63.40	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111819\
Data File : BF117826.D
Acq On : 18 Nov 2019 10:57
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 17:57:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

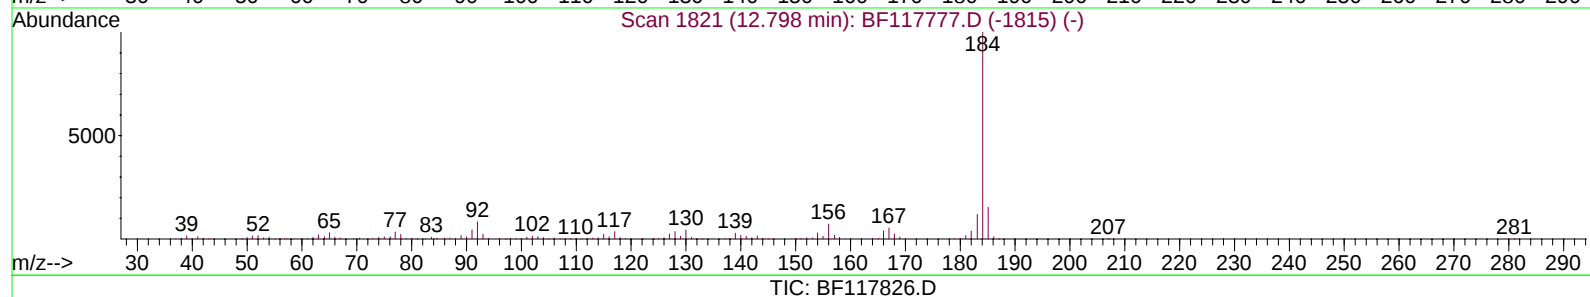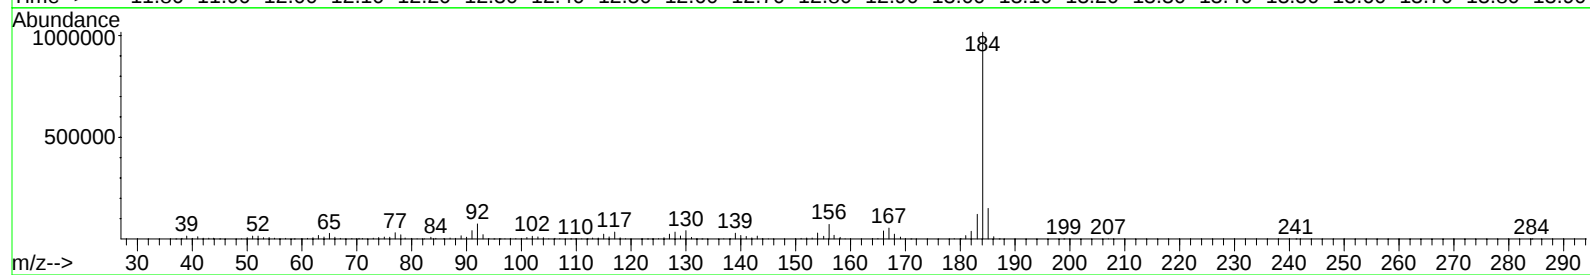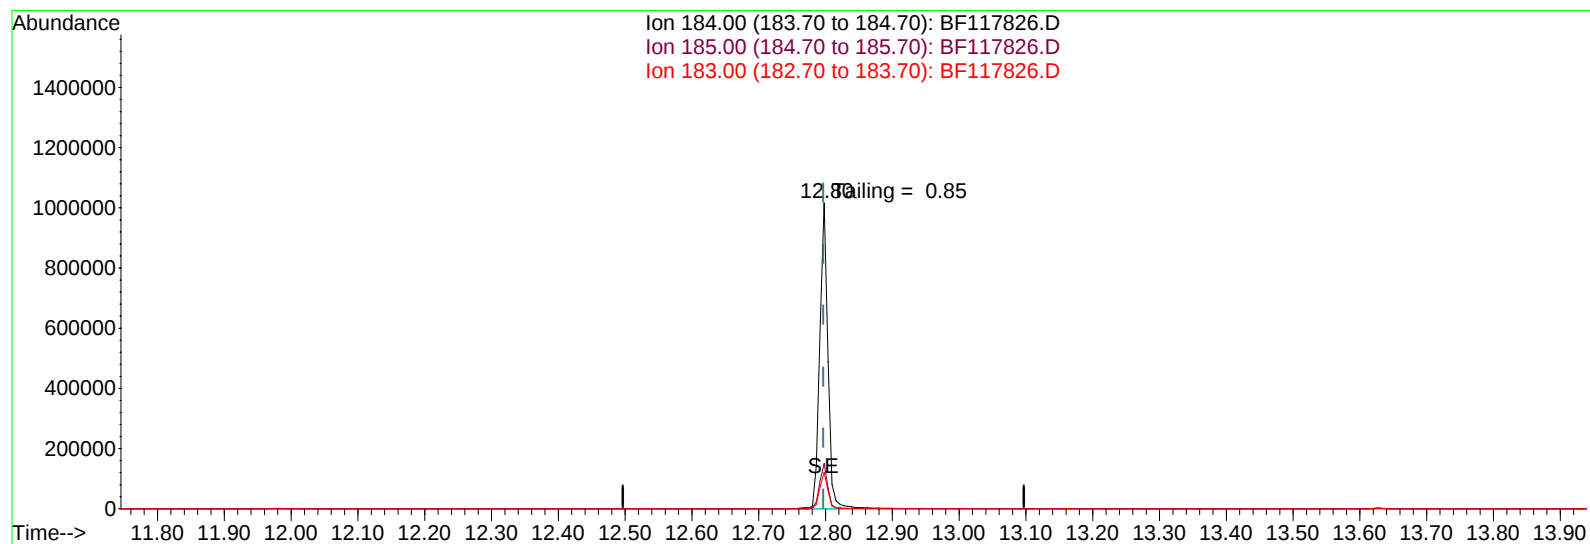

(77) Benzidine

12.798min (+0.001) 93023.07ng

response 868409

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.81
183.00	11.90	11.94
0.00	0.00	0.00