


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111819\
 Data File : BF117826.D
 Acq On : 18 Nov 2019 10:57
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

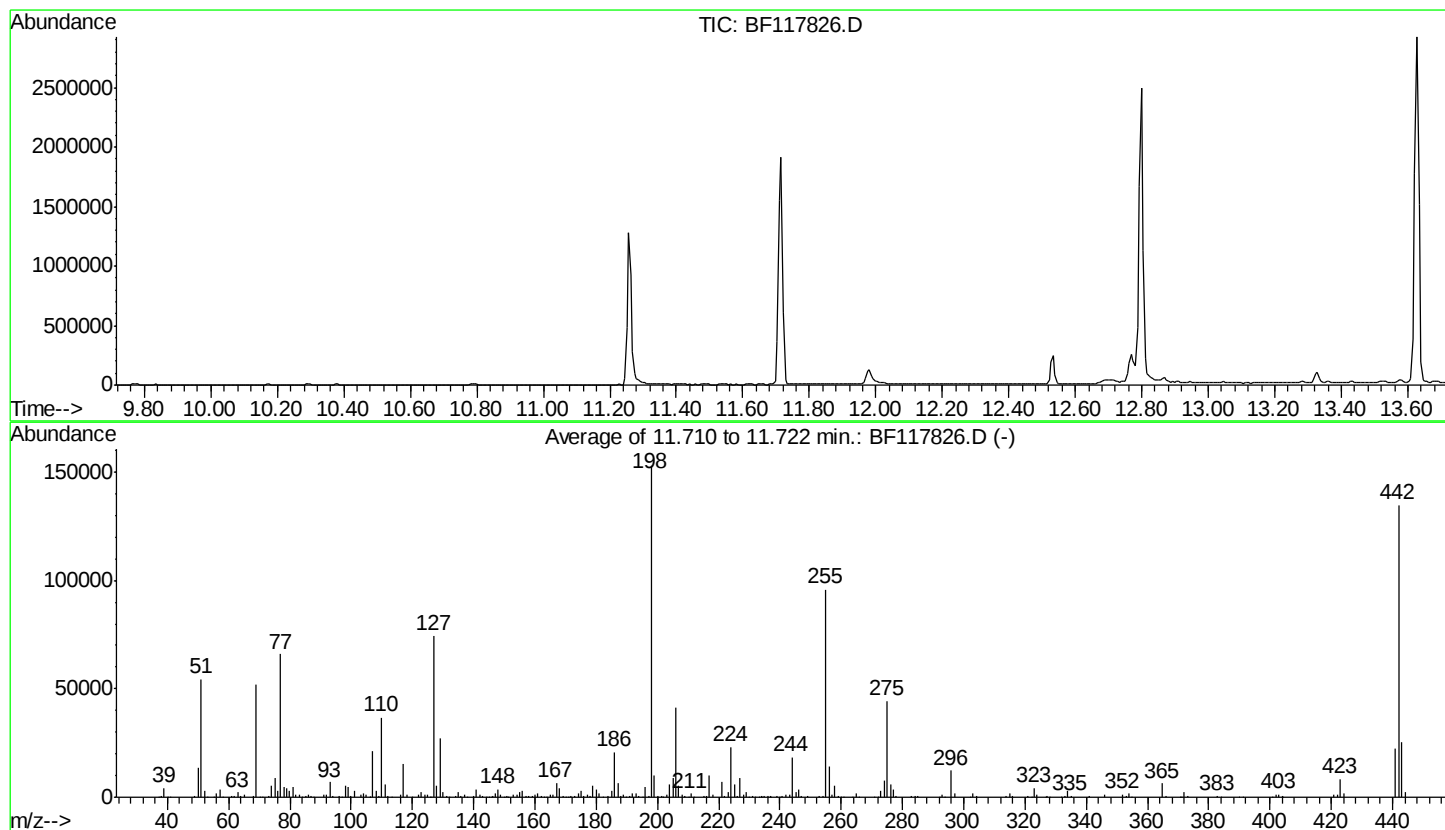

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	54417	PASS
68	69	0.00	2	1.7	865	PASS
69	198	0.00	100	34.1	52148	PASS
70	69	0.00	2	0.6	308	PASS
127	198	10	80	48.8	74677	PASS
197	198	0.00	2	0.4	687	PASS
198	198	100	100	100.0	152949	PASS
199	198	5	9	6.4	9853	PASS
275	198	10	60	29.0	44416	PASS
365	198	1	100	4.2	6355	PASS
441	198	0.01	100	14.6	22380	PASS
442	198	50	100	88.1	134717	PASS
443	442	15	24	19.0	25586	PASS