
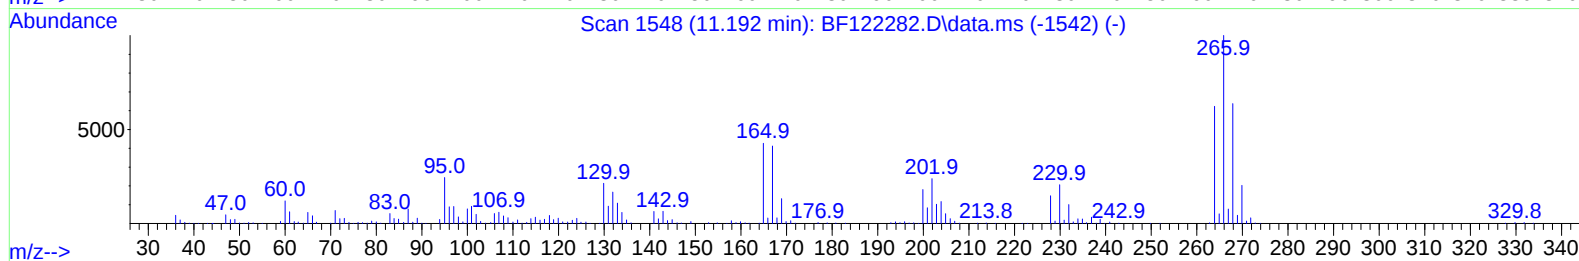
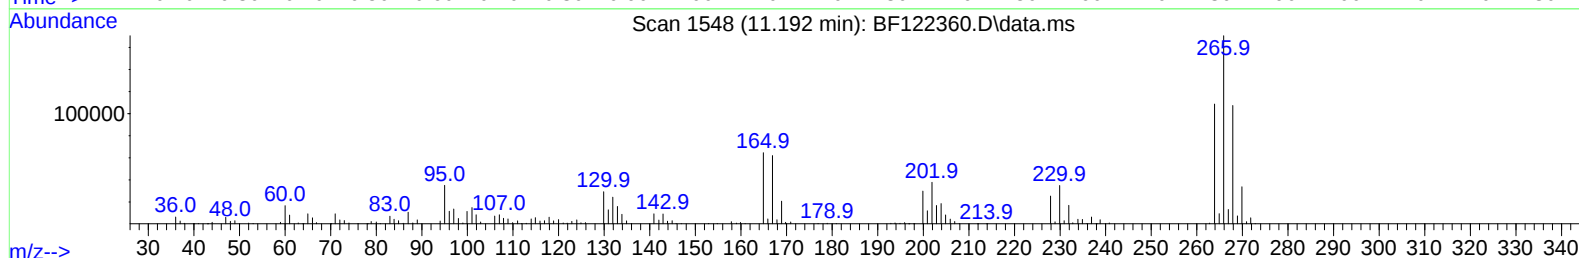


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111820\
Data File : BF122360.D
Acq On : 18 Nov 2020 10:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 02:20:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

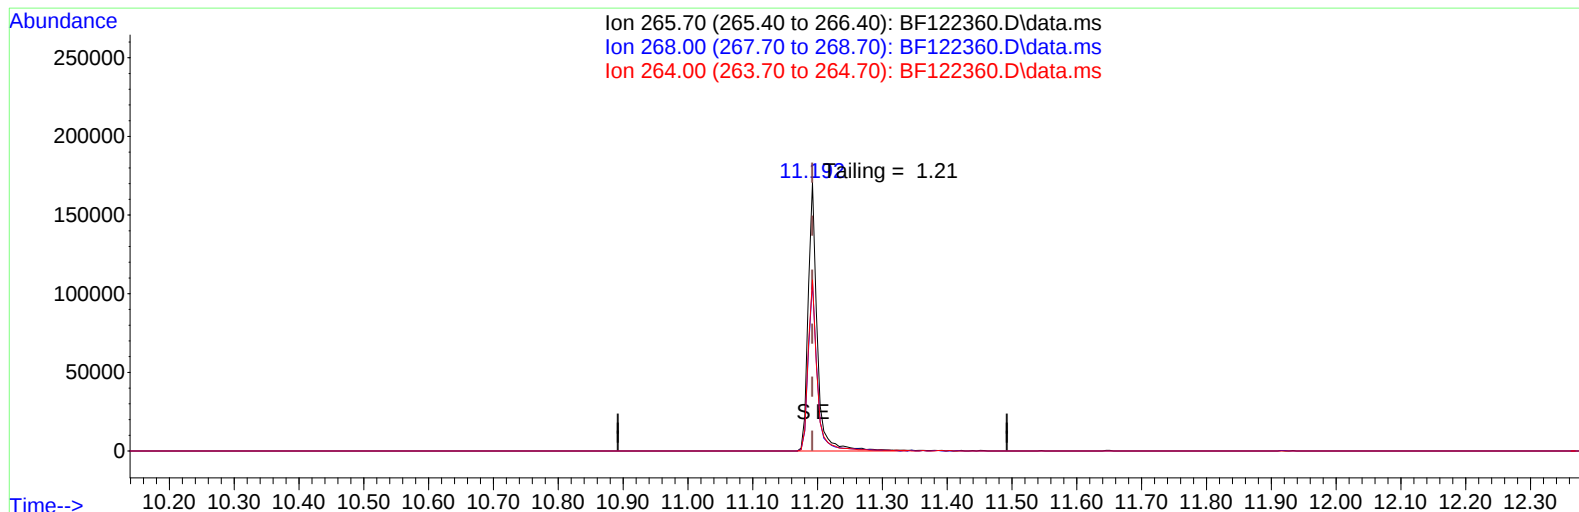

TIC: BF122360.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 35265.84 ng

response 167674

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	62.97
264.00	62.40	63.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111820\
Data File : BF122360.D
Acq On : 18 Nov 2020 10:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 02:20:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

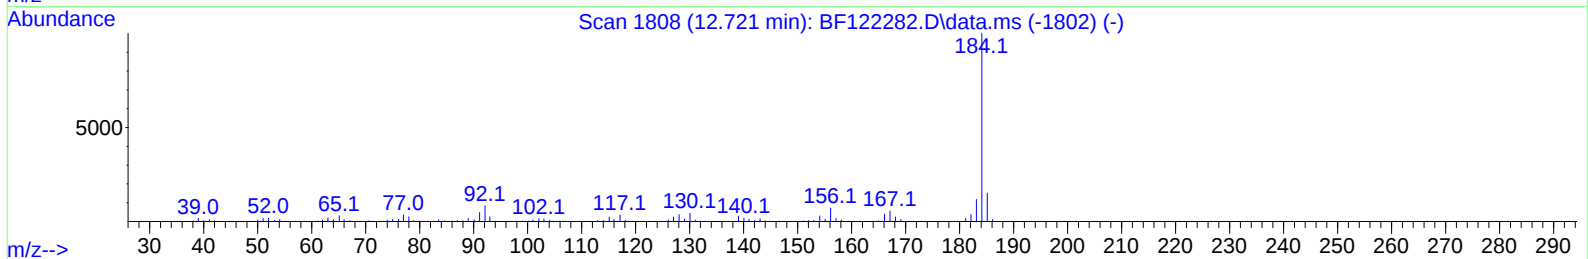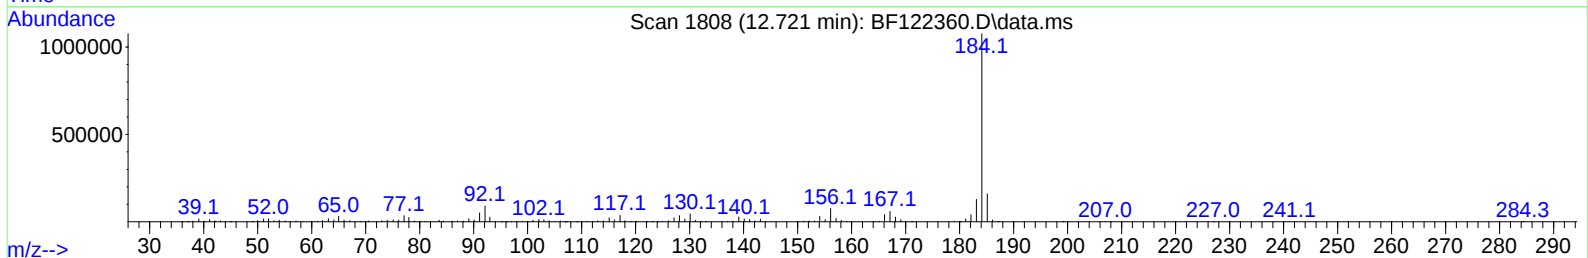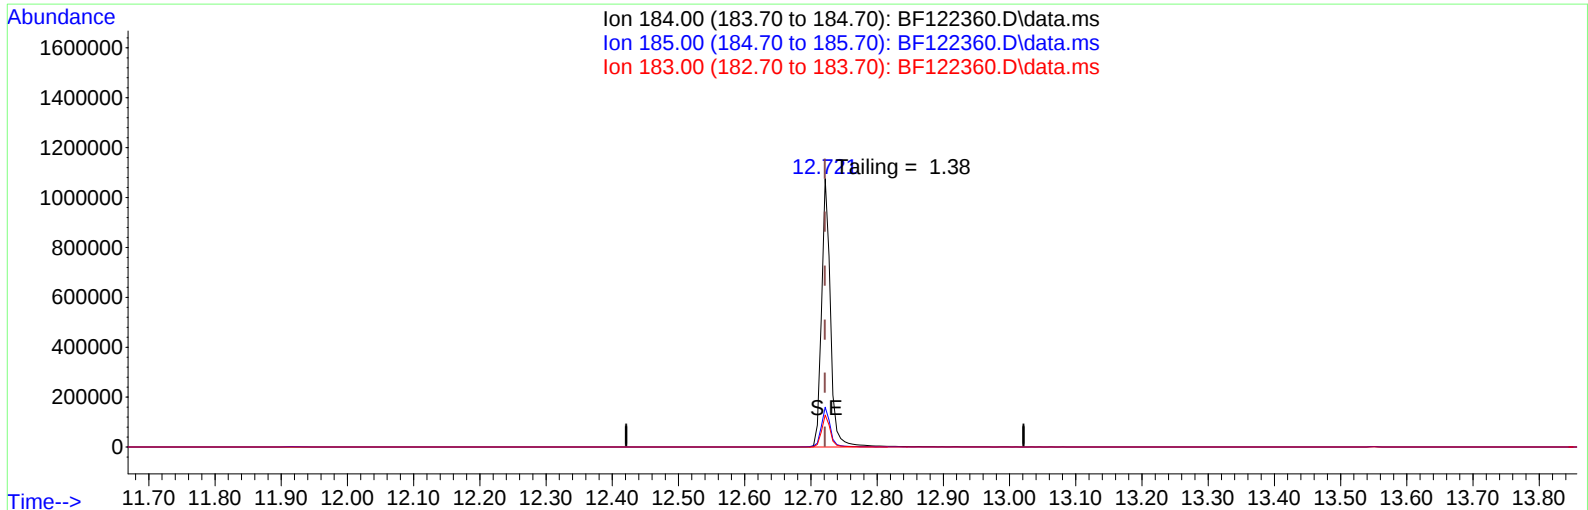

TIC: BF122360.D\data.ms

(77) Benzidine

12.721min (+ 0.000) 0.00 ng

response 1009506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.85
183.00	11.70	11.92
0.00	0.00	0.00