


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111820\  
Data File : BF122360.D  
Acq On : 18 Nov 2020 10:58  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110920.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Nov 10 12:25:42 2020

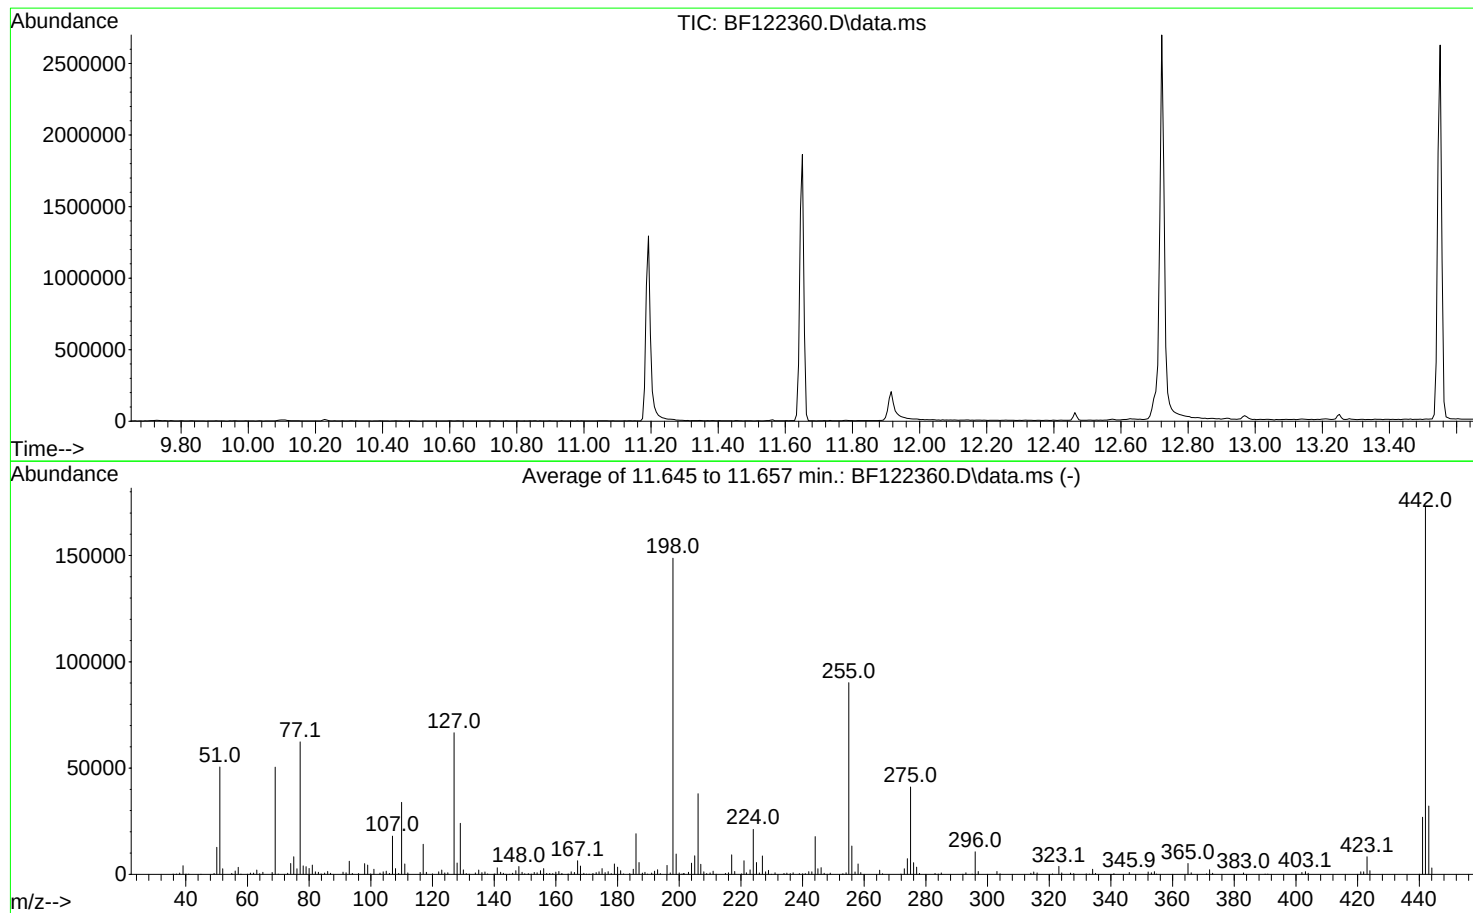

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.0         | 50516      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 872        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.9         | 50457      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 148        | PASS                |
| 127            | 198             | 10              | 80              | 44.8         | 66589      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 654        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 148779     | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 9594       | PASS                |
| 275            | 198             | 10              | 60              | 27.6         | 41088      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 5115       | PASS                |
| 441            | 198             | 0.01            | 100             | 18.1         | 26877      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 173064     | PASS                |
| 443            | 442             | 15              | 24              | 18.6         | 32141      | PASS                |