
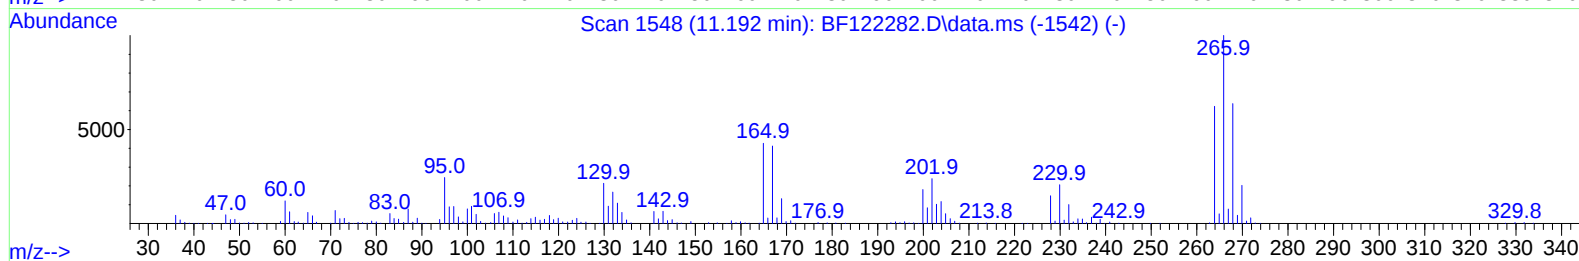
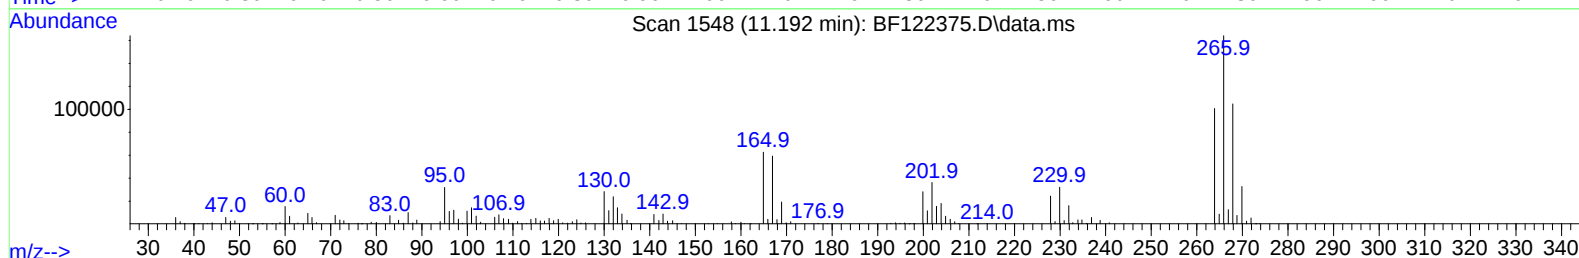


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111920\  
Data File : BF122375.D  
Acq On    : 19 Nov 2020  12:01  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 20 08:04:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

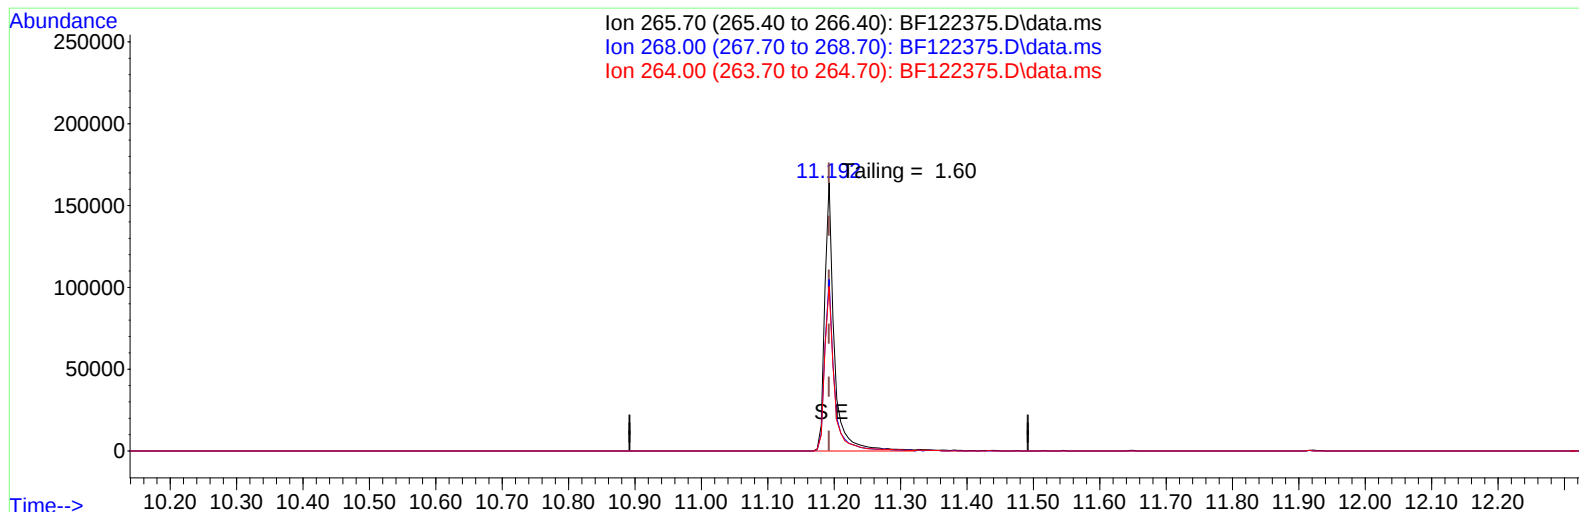

TIC: BF122375.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 45033.26 ng

response **164703**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	63.85
264.00	62.40	61.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111920\
Data File : BF122375.D
Acq On : 19 Nov 2020 12:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 08:04:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

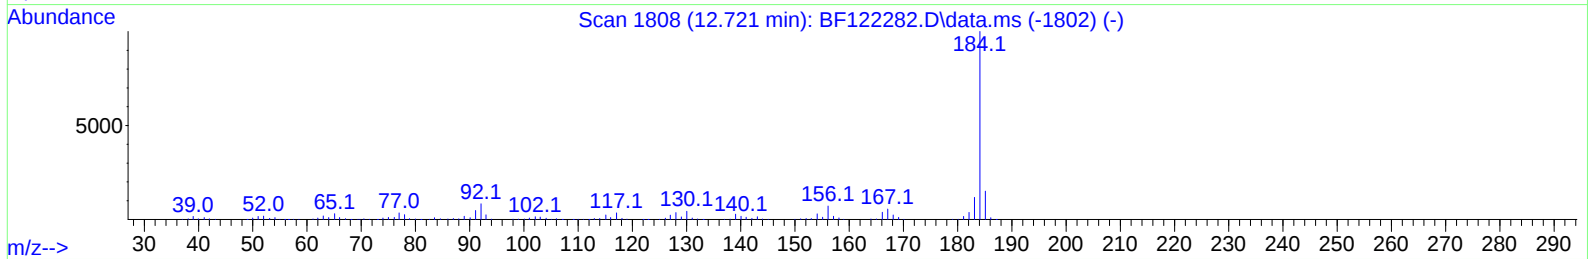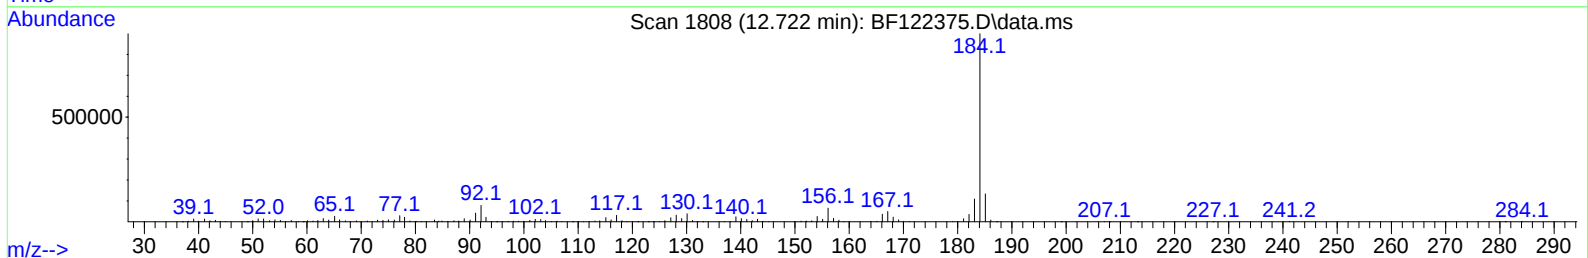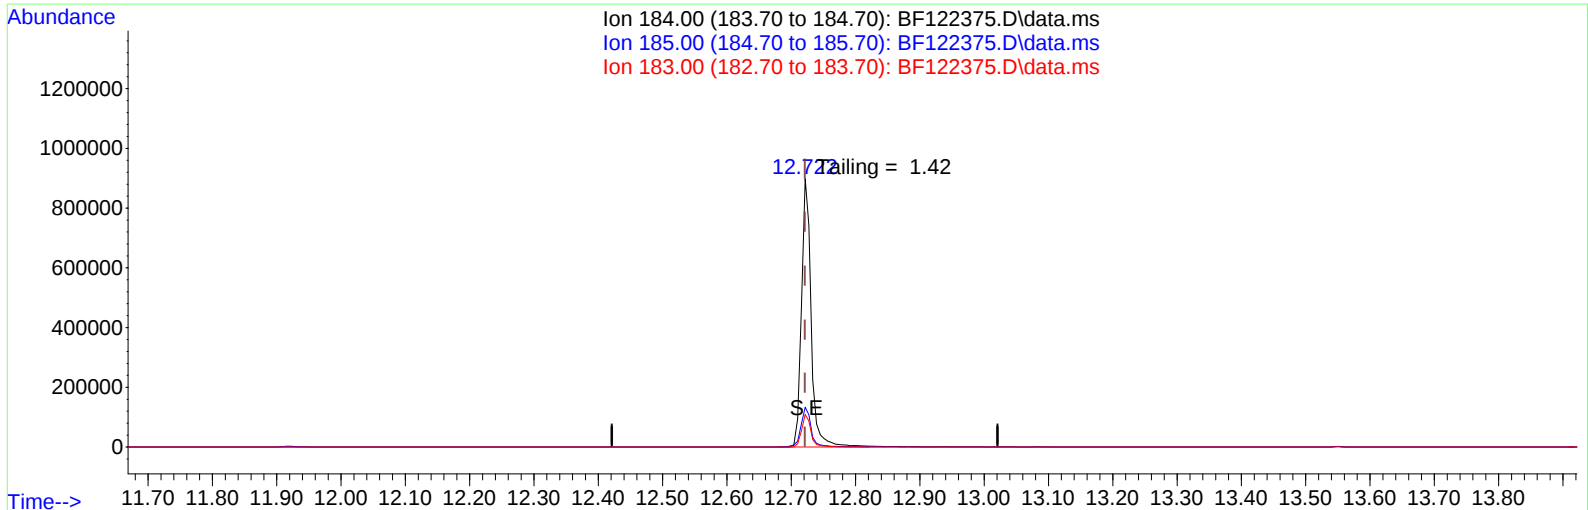

TIC: BF122375.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 0.00 ng

response 949227

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.84
183.00	11.70	12.10
0.00	0.00	0.00