
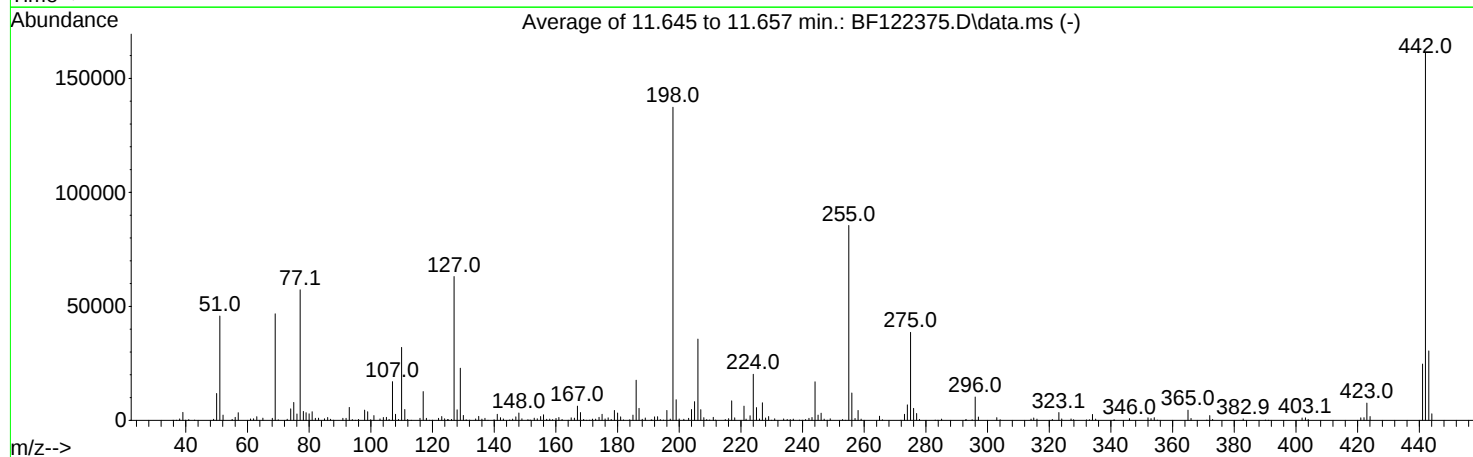


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111920\
Data File : BF122375.D
Acq On : 19 Nov 2020 12:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 20 13:27:02 2020

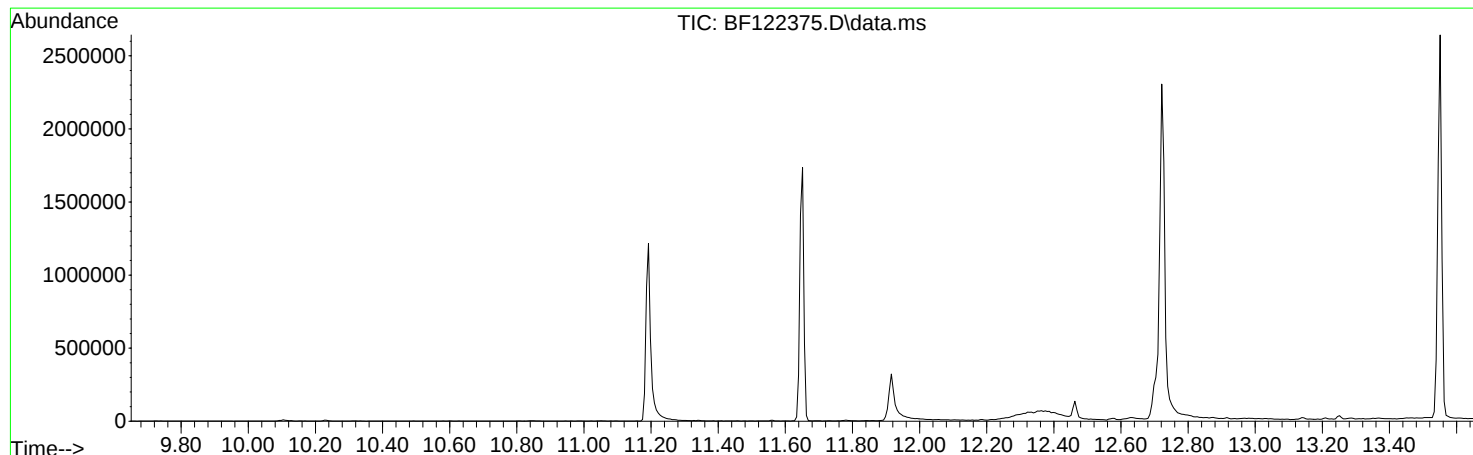

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	45775	PASS
68	69	0.00	2	1.9	911	PASS
69	198	0.00	100	34.0	46741	PASS
70	69	0.00	2	0.6	266	PASS
127	198	10	80	45.9	63067	PASS
197	198	0.00	2	0.4	570	PASS
198	198	100	100	100.0	137349	PASS
199	198	5	9	6.6	9033	PASS
275	198	10	60	28.1	38619	PASS
365	198	1	100	3.3	4524	PASS
441	198	0.01	100	18.0	24680	PASS
442	442	100	100	100.0	161355	PASS
443	442	15	24	18.9	30451	PASS