

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111925\  
 Data File : BF144276.D  
 Acq On : 19 Nov 2025 13:07  
 Operator : RC/JU  
 Sample : PB170631BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB170631BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144276.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.099       | 487           | 494         | 513          | rBV      | 274293         | 440492        | 25.55%          | 4.064%        |
| 2         | 5.499       | 557           | 562         | 588          | rBV      | 1052288        | 1408610       | 81.69%          | 12.996%       |
| 3         | 6.498       | 726           | 732         | 754          | rBV      | 1031234        | 1417930       | 82.23%          | 13.082%       |
| 4         | 6.869       | 790           | 795         | 808          | rVB      | 246882         | 317107        | 18.39%          | 2.926%        |
| 5         | 7.428       | 884           | 890         | 904          | rBV      | 684077         | 910301        | 52.79%          | 8.399%        |
| 6         | 8.145       | 1007          | 1012        | 1027         | rBV      | 299349         | 403720        | 23.41%          | 3.725%        |
| 7         | 9.222       | 1190          | 1195        | 1207         | rBV      | 1278370        | 1724374       | 100.00%         | 15.910%       |
| 8         | 9.904       | 1306          | 1311        | 1321         | rBV      | 364073         | 465508        | 27.00%          | 4.295%        |
| 9         | 10.698      | 1441          | 1446        | 1463         | rBV      | 808688         | 1065125       | 61.77%          | 9.827%        |
| 10        | 11.398      | 1559          | 1565        | 1572         | rBV      | 330216         | 429832        | 24.93%          | 3.966%        |
| 11        | 12.986      | 1829          | 1835        | 1840         | rBV      | 1072961        | 1426247       | 82.71%          | 13.159%       |
| 12        | 14.045      | 2010          | 2015        | 2023         | rBV      | 240251         | 315260        | 18.28%          | 2.909%        |
| 13        | 15.527      | 2261          | 2267        | 2276         | rBV      | 230730         | 371979        | 21.57%          | 3.432%        |
| 14        | 17.192      | 2542          | 2550        | 2566         | rVB2     | 34679          | 142081        | 8.24%           | 1.311%        |




Sum of corrected areas: 10838566

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111925\  
Data File : BF144276.D  
Acq On : 19 Nov 2025 13:07  
Operator : RC/JU  
Sample : PB170631BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB170631BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

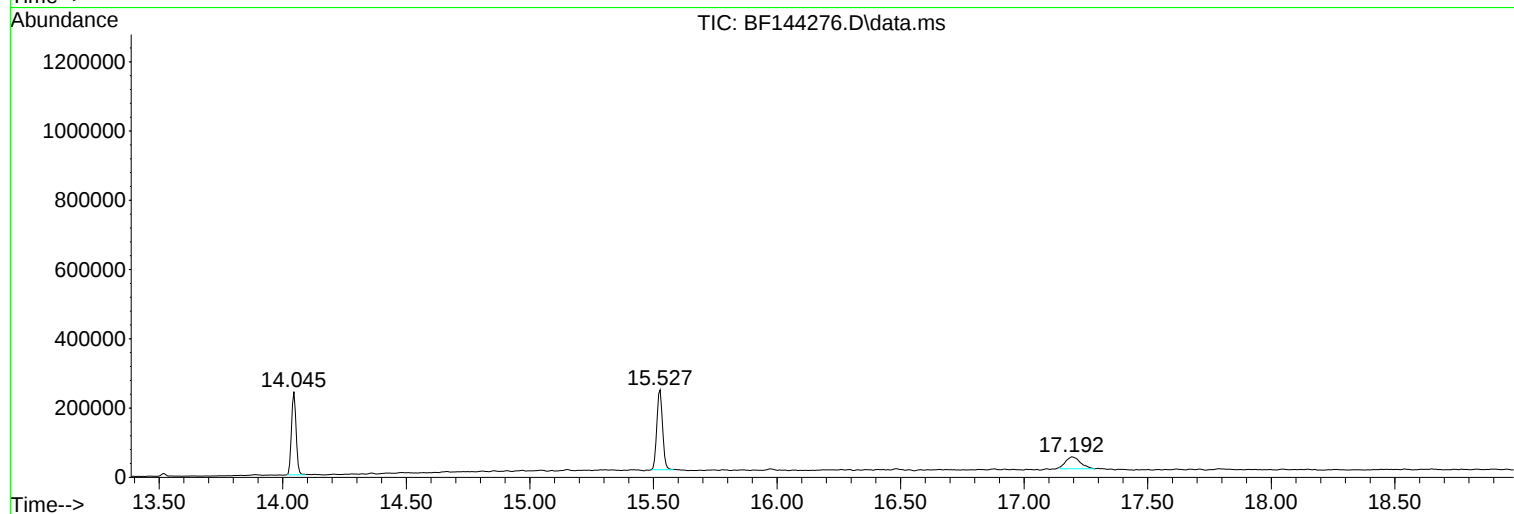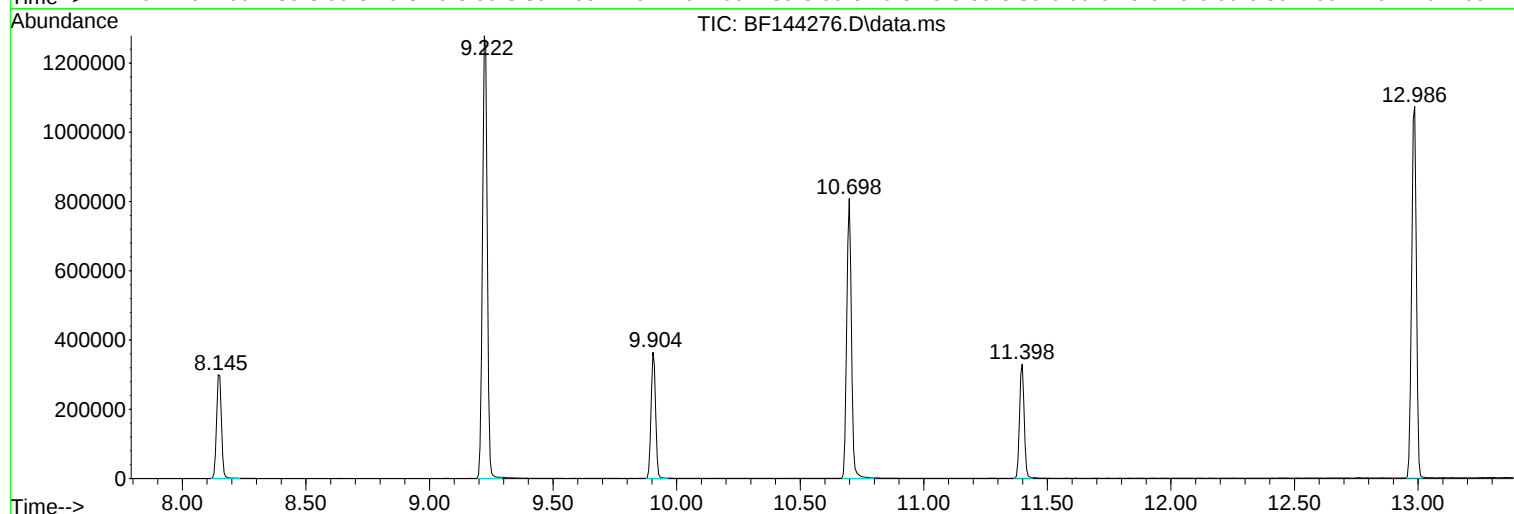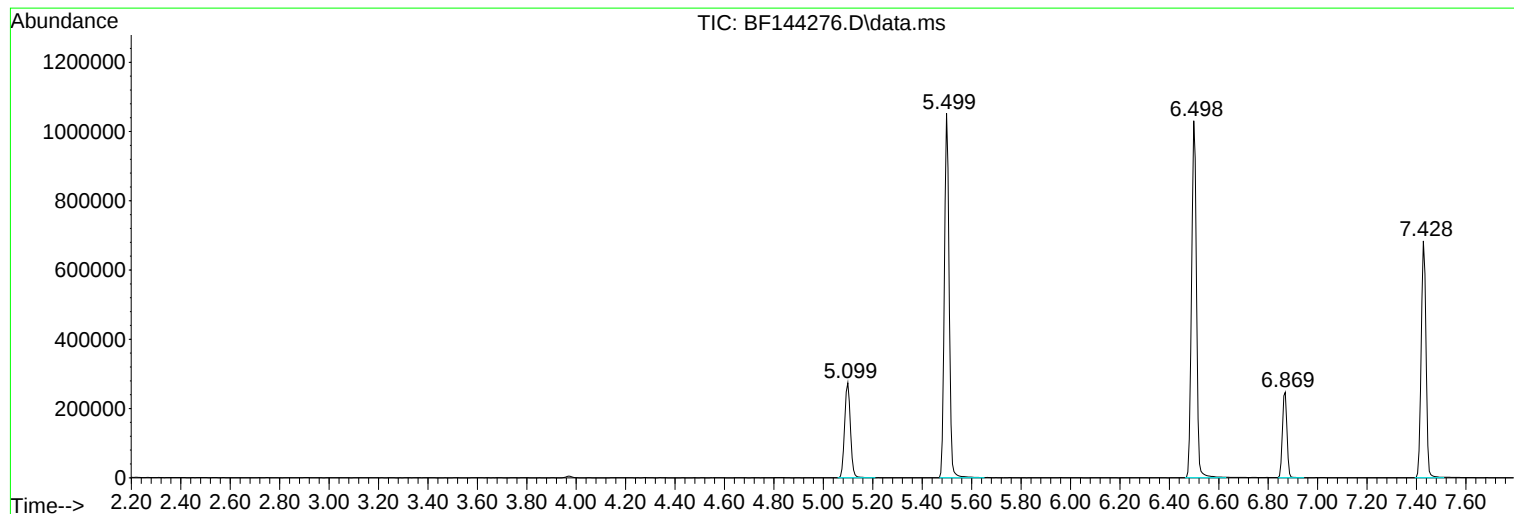

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111925\  
Data File : BF144276.D  
Acq On : 19 Nov 2025 13:07  
Operator : RC/JU  
Sample : PB170631BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB170631BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111925\  
Data File : BF144276.D  
Acq On : 19 Nov 2025 13:07  
Operator : RC/JU  
Sample : PB170631BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB170631BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|