
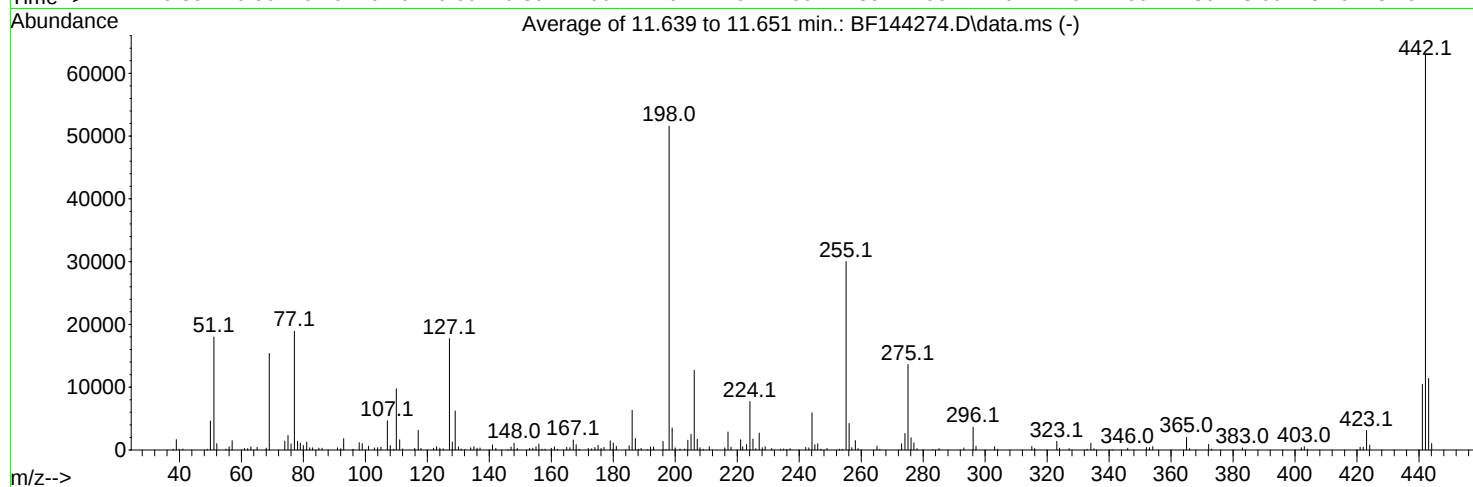


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111925\
Data File : BF144274.D
Acq On : 19 Nov 2025 12:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

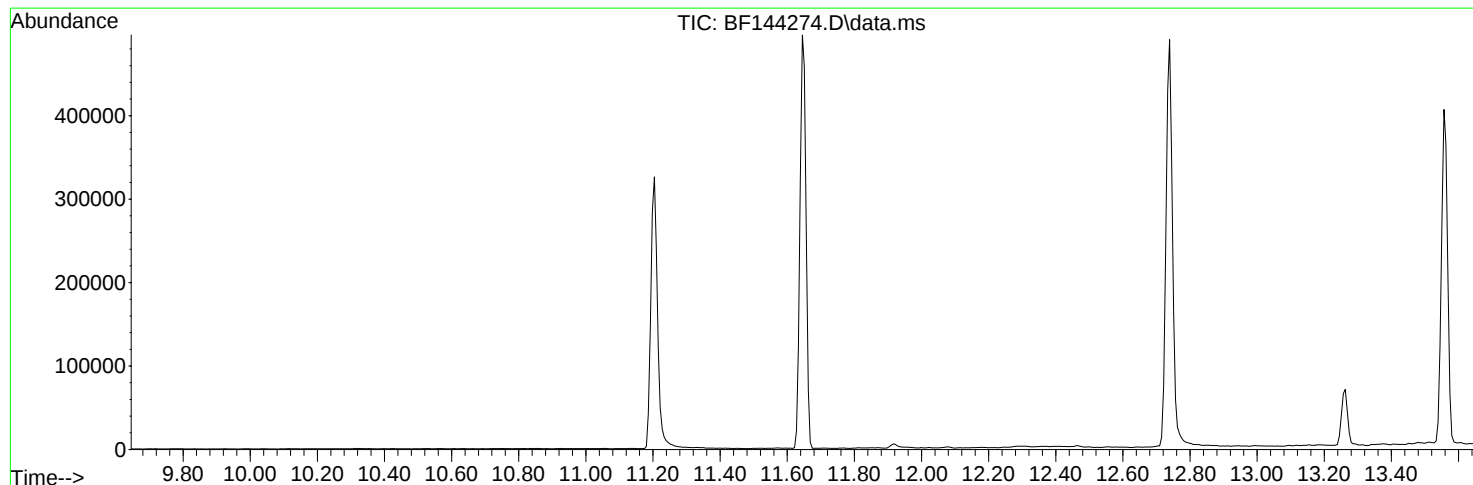


AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	298	PASS
69	69	100	100	100.0	15397	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.1	57	PASS
198	198	100	100	100.0	51581	PASS
199	198	5	9	6.8	3510	PASS
365	198	1	100	3.9	2026	PASS
441	443	0.01	150	92.0	10479	PASS
442	442	100	100	100.0	62901	PASS
443	442	15	24	18.1	11385	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111925\
Data File : BF144274.D
Acq On : 19 Nov 2025 12:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 19 12:47:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

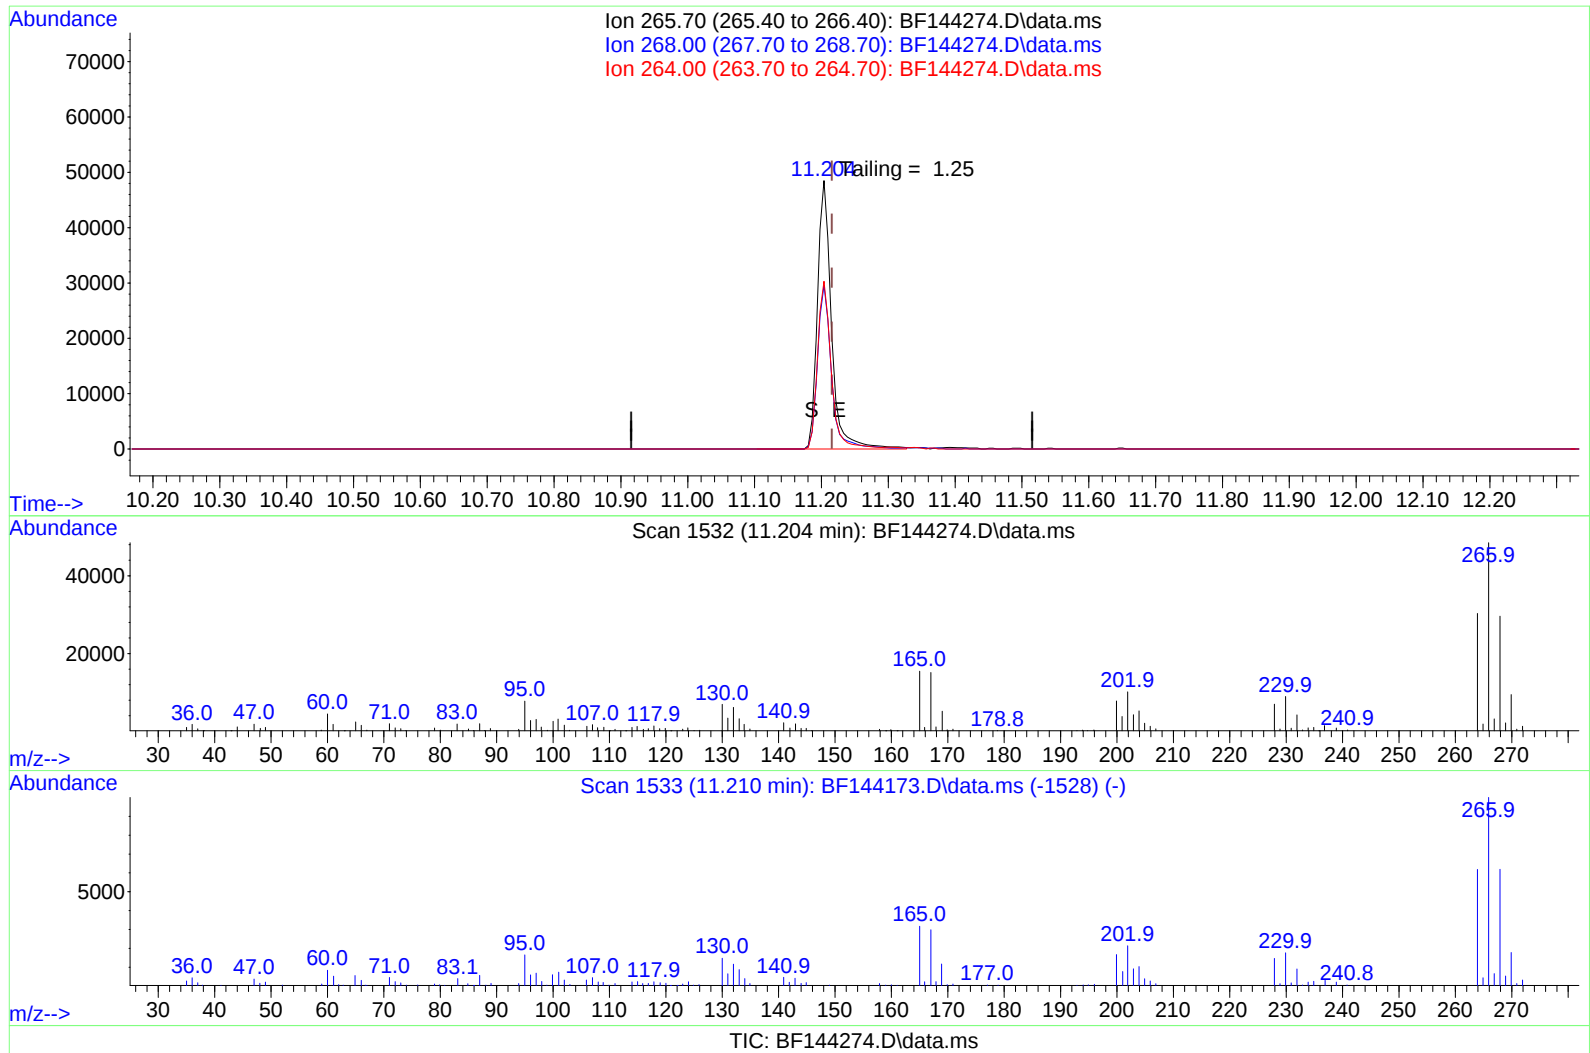

(70) Pentachlorophenol (C)

11.204min (-0.012) 76530.83 ng




response 71046

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.09
264.00	61.80	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111925\
Data File : BF144274.D
Acq On : 19 Nov 2025 12:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 19 12:47:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

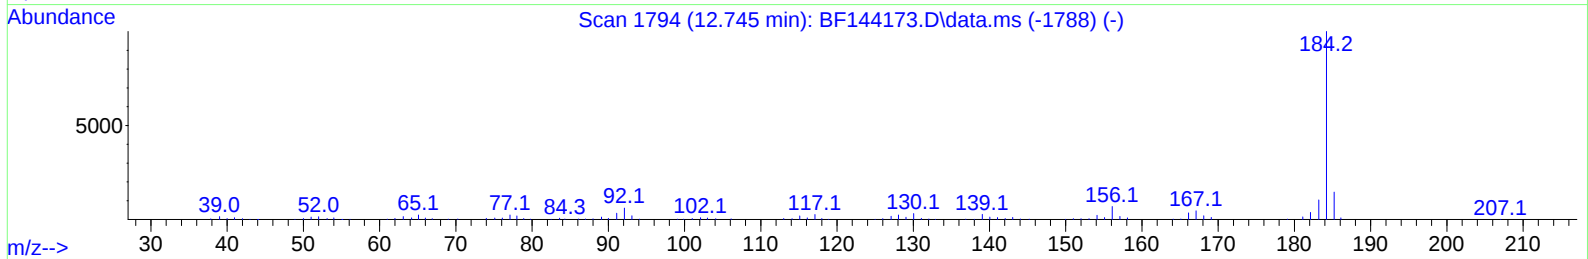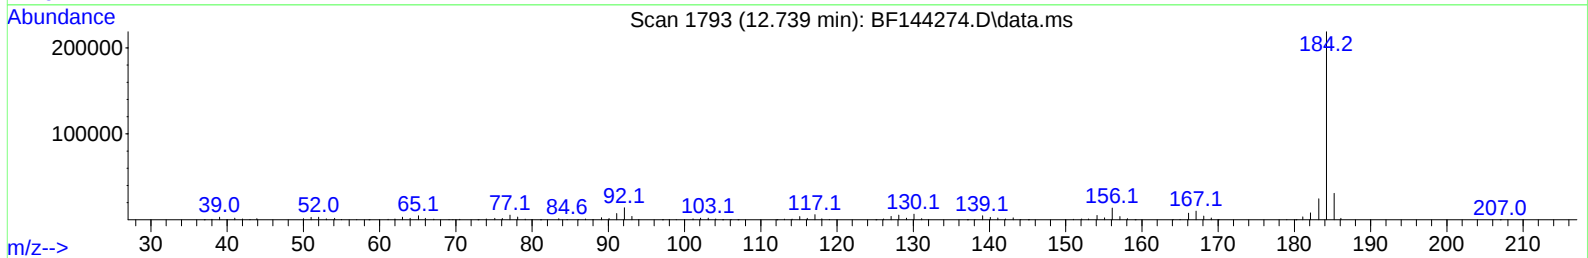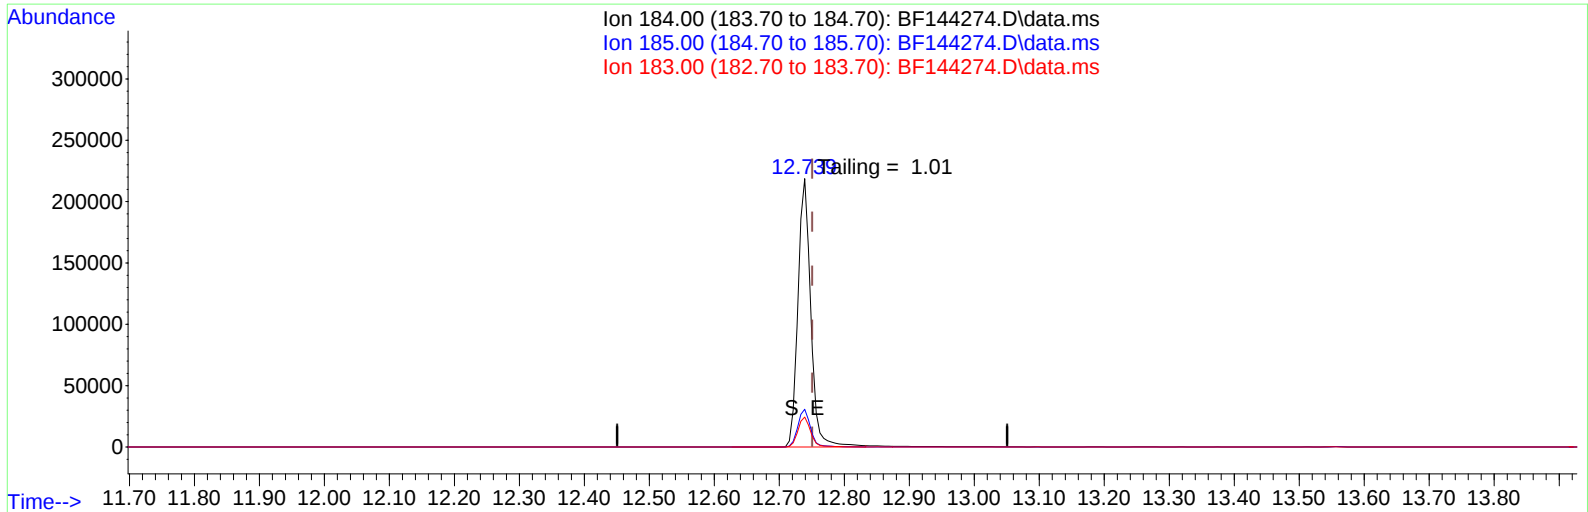

TIC: BF144274.D\data.ms

(77) Benzidine

12.739min (-0.012) 0.00 ng

response 304116

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.11
183.00	10.40	11.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2025	BNA_F	<u>BF144274.D</u>
Compound Name	Response	Retention Time
DDT	112538	13.557
DDD		13.263
DDE	1415	11.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1415	113953	1.24

Instrument :
BNA_F
ClientSampleId :
DFTPP