

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
 Data File : BF140507.D
 Acq On : 20 Nov 2024 18:43
 Operator : RC/JU
 Sample : P4893-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 21 00:07:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 14:40:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	100112	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	364052	20.000	ng	0.00
39) Acenaphthene-d10	9.904	164	187678	20.000	ng	-0.01
64) Phenanthrene-d10	11.398	188	315574	20.000	ng	0.00
76) Chrysene-d12	14.039	240	202306	20.000	ng	-0.01
86) Perylene-d12	15.533	264	204013	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	474189	80.872	ng	0.01
7) Phenol-d6	6.510	99	614848	77.397	ng	0.00
23) Nitrobenzene-d5	7.434	82	392498	56.174	ng	0.00
42) 2,4,6-Tribromophenol	10.698	330	137727	73.796	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	680255	58.267	ng	-0.01
79) Terphenyl-d14	12.980	244	546390	46.880	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.434	70	51156	10.662	ng	# 76
25) Isophorone	7.434	82	392123	31.665	ng	# 66
51) 2,6-Dinitrotoluene	9.904	165	24508	8.788	ng	# 22
57) 2,4-Dinitrotoluene	9.904	165	24508	6.677	ng	# 20
63) Azobenzene	10.616	77	34775	2.814	ng	# 1
67) 4-Bromophenyl-phenylether	10.698	248	8571	2.717	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140507.D
Acq On : 20 Nov 2024 18:43
Operator : RC/JU
Sample : P4893-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :


Quant Time: Nov 21 00:07:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

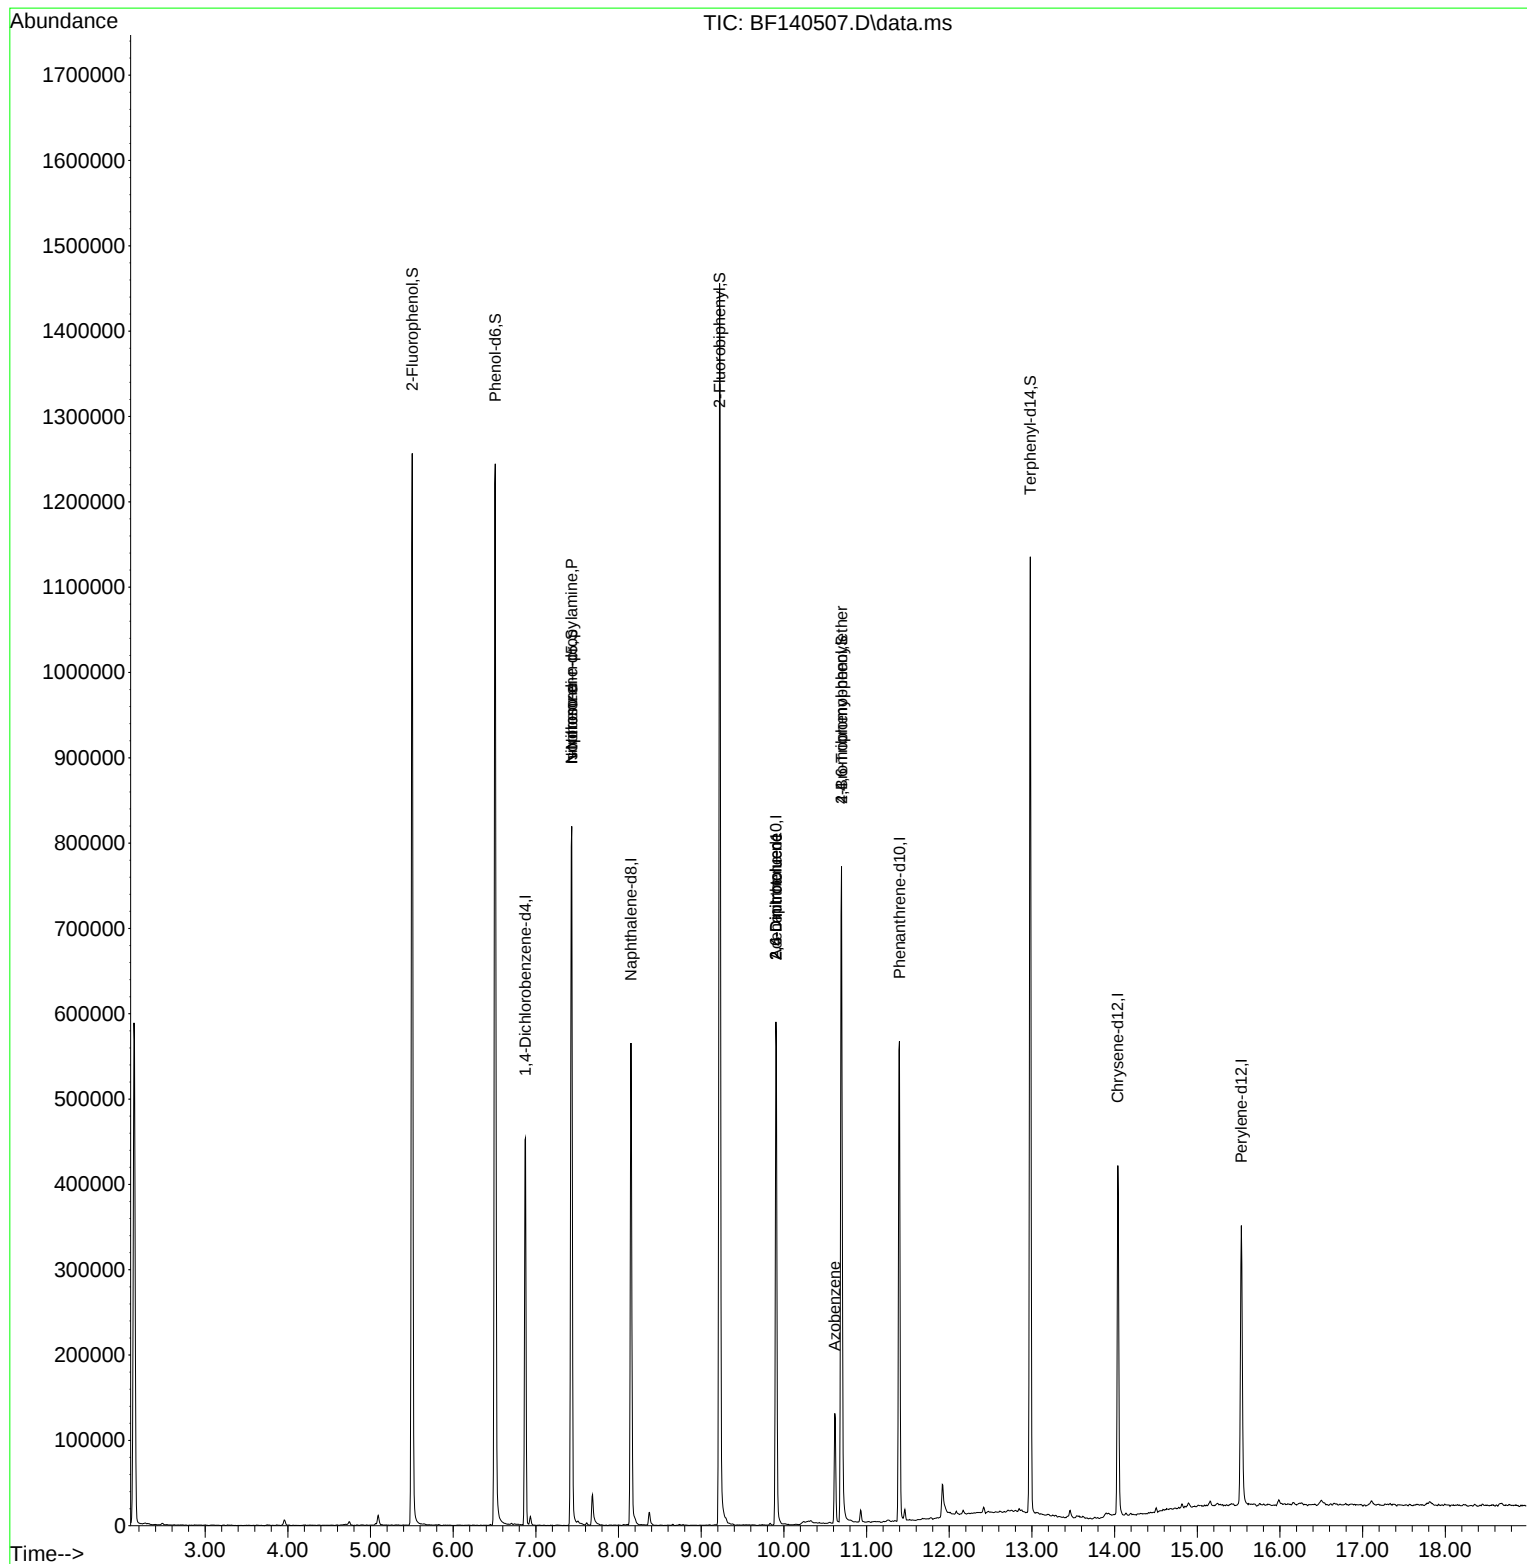






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43


Instrument :
BNA_F
ClientSampleId :

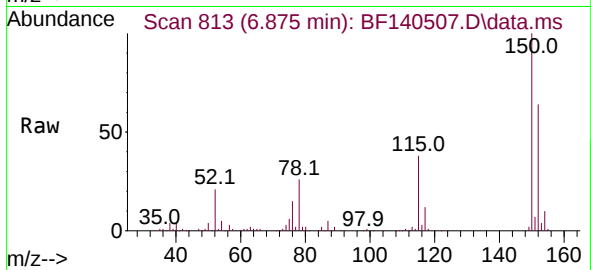



Tgt Ion:152 Resp: 100112
Ion Ratio Lower Upper
152 100
150 156.3 127.4 191.0
115 59.4 47.4 71.2

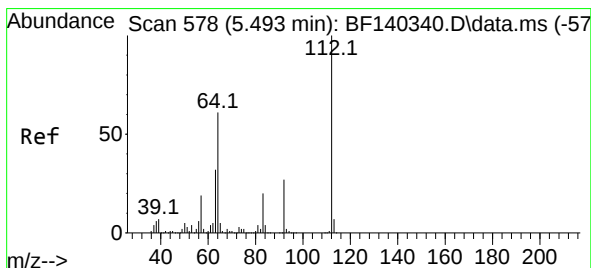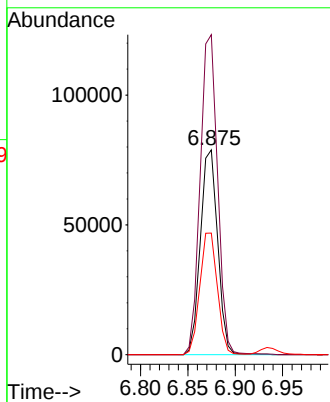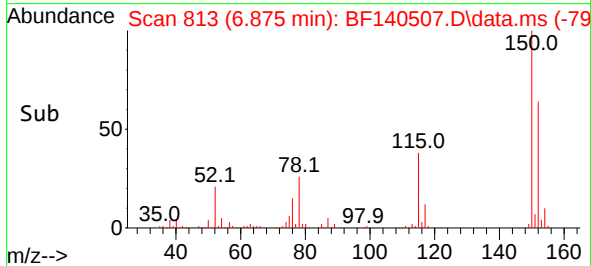

#5
2-Fluorophenol
Concen: 80.872 ng
RT: 5.504 min Scan# 580
Delta R.T. 0.012 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

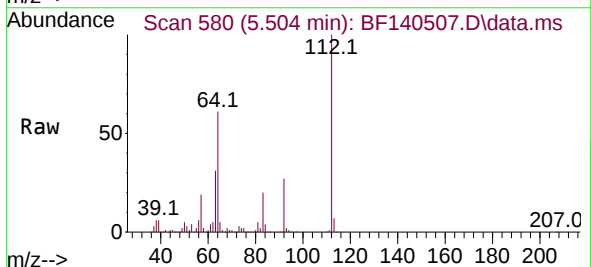


Tgt Ion:112 Resp: 474189
Ion Ratio Lower Upper
112 100
64 60.6 49.2 73.8
63 31.2 25.6 38.4

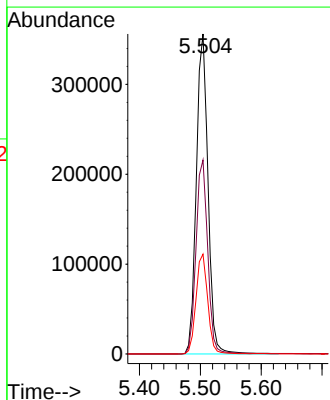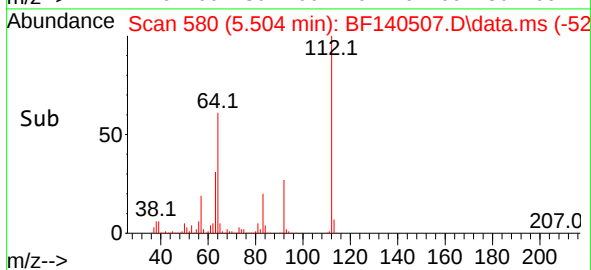





#7
Phenol-d6
Concen: 77.397 ng
RT: 6.510 min Scan# 71
Delta R.T. 0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

Instrument :
BNA_F
ClientSampleId :






Tgt Ion: 99 Resp: 614848
Ion Ratio Lower Upper
99 100
42 17.5 15.1 22.7
71 34.6 27.9 41.9

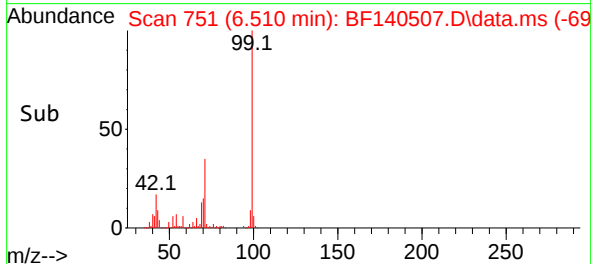

#19
n-Nitroso-di-n-propylamine
Concen: 10.662 ng
RT: 7.434 min Scan# 908
Delta R.T. 0.141 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

Tgt Ion: 70 Resp: 51156
Ion Ratio Lower Upper
70 100
42 45.1 46.8 70.2#
101 0.0 7.5 11.3#
130 1.9 16.3 24.5#

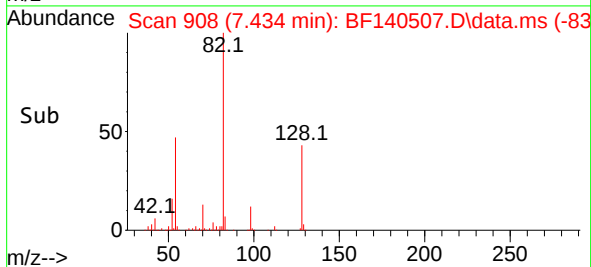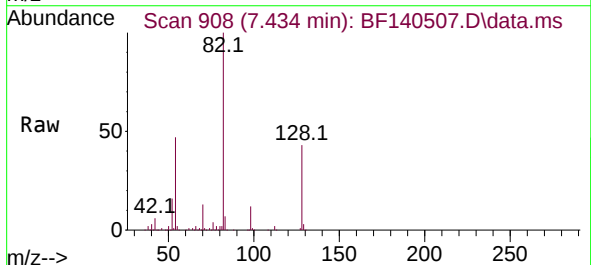




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43




Instrument :

BNA_F

ClientSampleId :







Tgt Ion:136 Resp: 364052
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 7.5 6.5 9.7
68 6.2 5.0 7.6

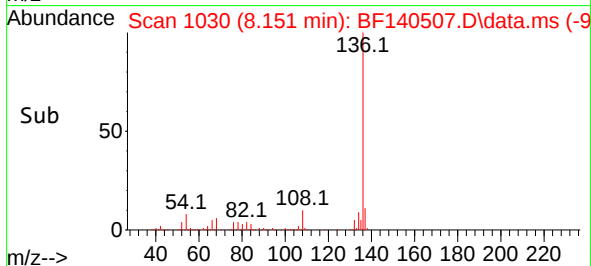

#23
Nitrobenzene-d5
Concen: 56.174 ng
RT: 7.434 min Scan# 908
Delta R.T. -0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

Tgt Ion: 82 Resp: 392498
Ion Ratio Lower Upper
82 100
128 43.2 33.3 49.9
54 47.4 39.8 59.8

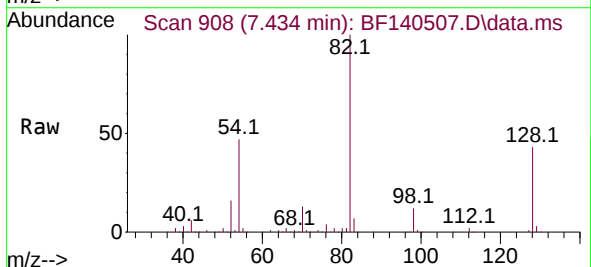



#25

Isophorone

Concen: 31.665 ng

RT: 7.434 min Scan# 90

Delta R.T. -0.265 min

Lab File: BF140507.D

Acq: 20 Nov 2024 18:43

Instrument :

BNA_F

ClientSampleId :





Tgt Ion: 82 Resp: 392123

Ion Ratio Lower Upper

82 100

95 0.0 5.9 8.9#

138 0.0 13.4 20.2#

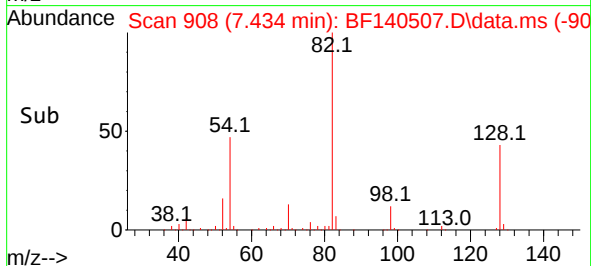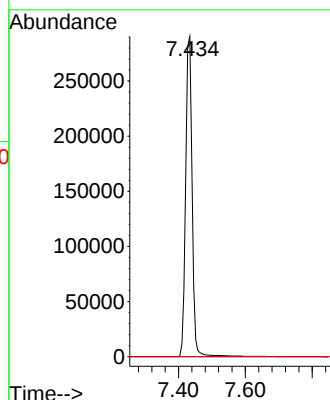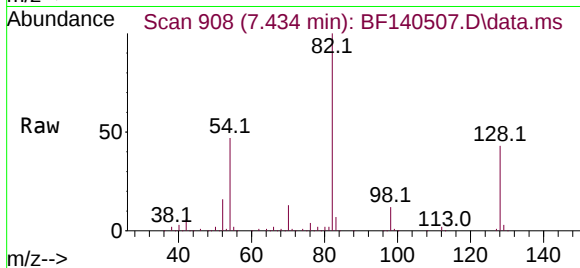

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.904 min Scan# 1328

Delta R.T. -0.012 min

Lab File: BF140507.D

Acq: 20 Nov 2024 18:43




Tgt Ion: 164 Resp: 187678


Ion Ratio Lower Upper

164 100

162 100.1 79.8 119.8


160 44.4 35.4 53.0

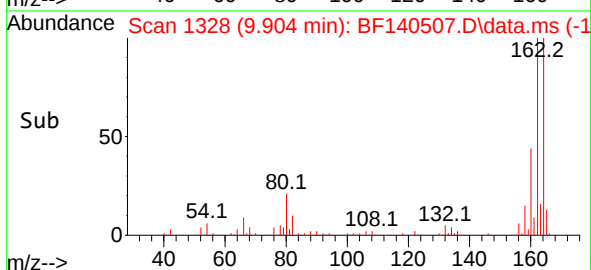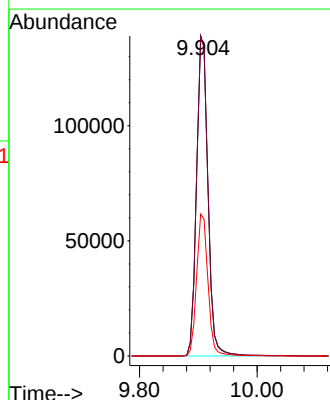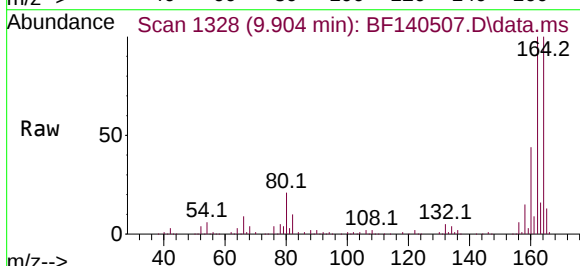






#42
2,4,6-Tribromophenol
Concen: 73.796 ng
RT: 10.698 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43


Instrument :
BNA_F
ClientSampleId :

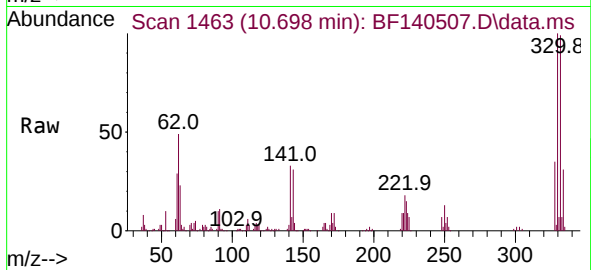



Tgt Ion:330 Resp: 137727
Ion Ratio Lower Upper
330 100
332 98.5 75.9 113.9
141 34.8 26.9 40.3

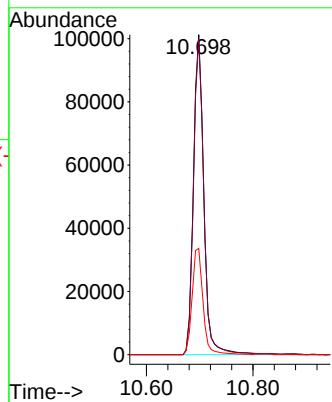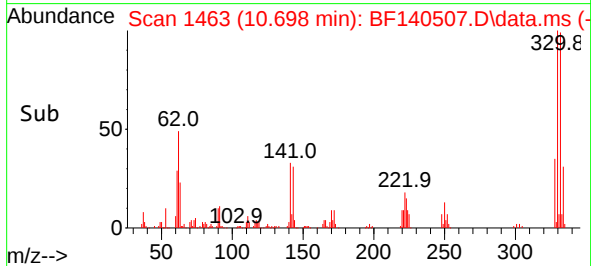


#45
2-Fluorobiphenyl
Concen: 58.267 ng
RT: 9.222 min Scan# 1212
Delta R.T. -0.012 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

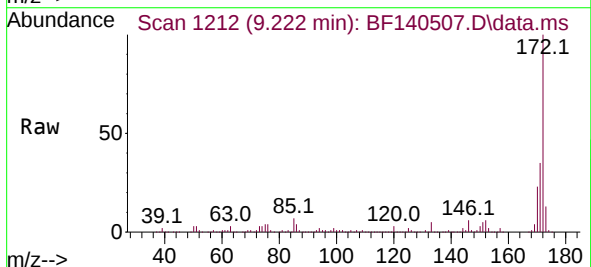

Tgt Ion:172 Resp: 680255
Ion Ratio Lower Upper
172 100
171 35.2 28.5 42.7
170 23.3 19.1 28.7



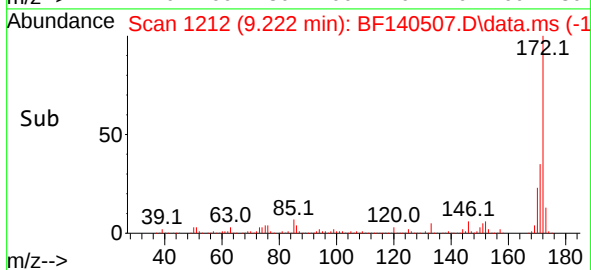




#51
2,6-Dinitrotoluene
Concen: 8.788 ng
RT: 9.904 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43




Instrument :
BNA_F
ClientSampleId :


Tgt Ion:165 Resp: 24508
Ion Ratio Lower Upper
165 100
63 1.2 47.6 71.4#
89 1.1 48.1 72.1#

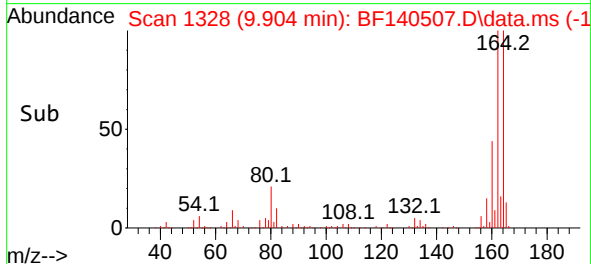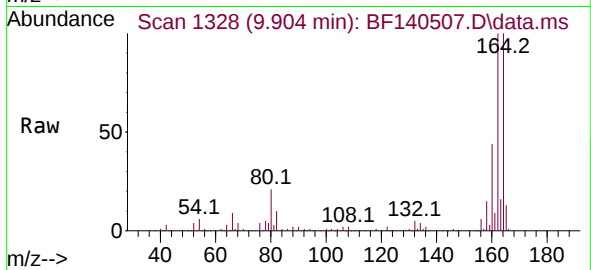

#57
2,4-Dinitrotoluene
Concen: 6.677 ng
RT: 9.904 min Scan# 1328
Delta R.T. -0.200 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43


Tgt Ion:165 Resp: 24508
Ion Ratio Lower Upper
165 100
63 1.2 39.4 59.0#
89 1.1 62.4 93.6#
182 0.0 2.1 3.1#

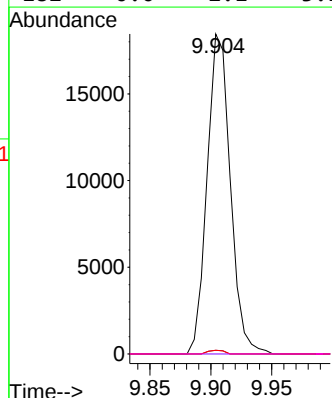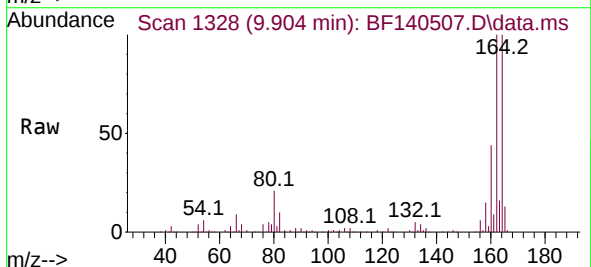



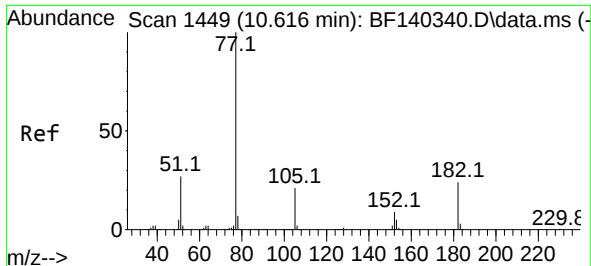


#63
Azobenzene
Concen: 2.814 ng
RT: 10.616 min Scan# 1449
Delta R.T. -0.000 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

Instrument :
BNA_F
ClientSampleId :







Tgt Ion: 77	Resp: 34775
Ion Ratio	Lower Upper
77	100
182	79.0 4.6 44.6#
105	153.9 0.9 40.9#
51	37.3 8.3 48.3

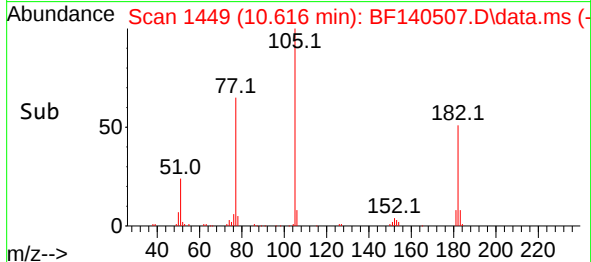

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 1582
Delta R.T. -0.006 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43

Tgt Ion: 188	Resp: 315574
Ion Ratio	Lower Upper
188	100
94	9.1 7.6 11.4
80	9.4 8.0 12.0


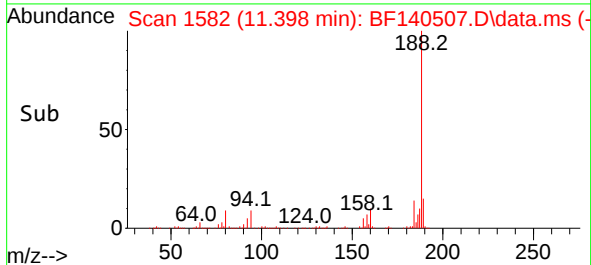

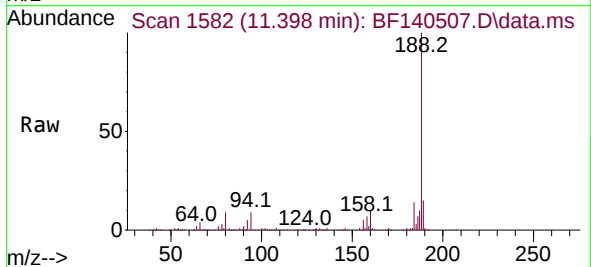




#67
4-Bromophenyl-phenylether
Concen: 2.717 ng
RT: 10.698 min Scan# 14
Delta R.T. -0.247 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43




Instrument :
BNA_F
ClientSampleId :


Tgt Ion:248 Resp: 8571
Ion Ratio Lower Upper
248 100
250 199.7 77.9 116.9#
141 506.3 61.8 92.6#

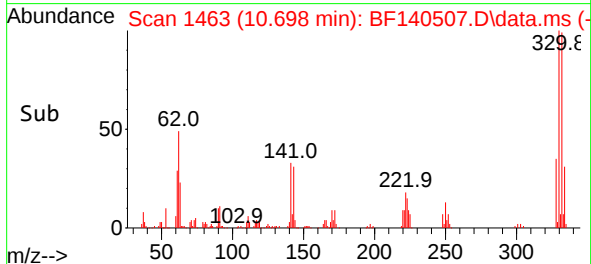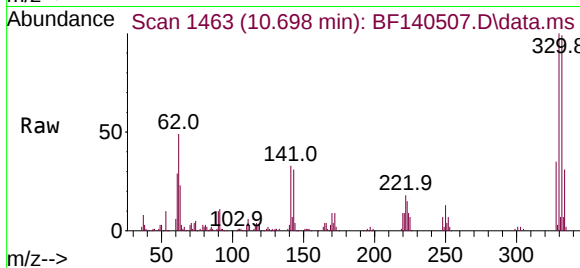

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2031
Delta R.T. -0.012 min
Lab File: BF140507.D
Acq: 20 Nov 2024 18:43


Tgt Ion:240 Resp: 202306
Ion Ratio Lower Upper
240 100
120 11.1 8.8 13.2
236 25.3 20.9 31.3

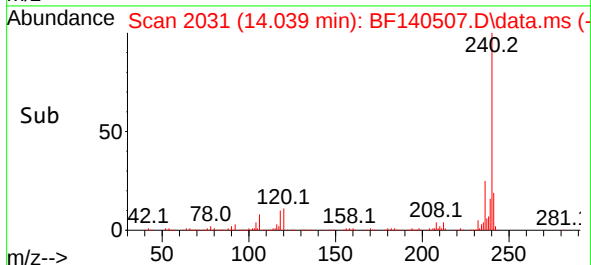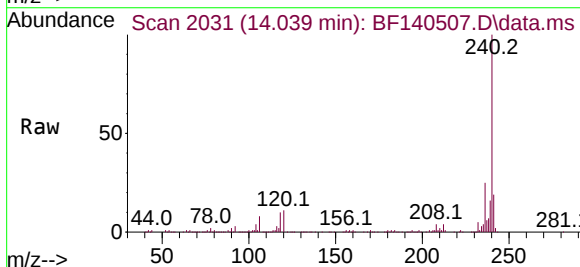



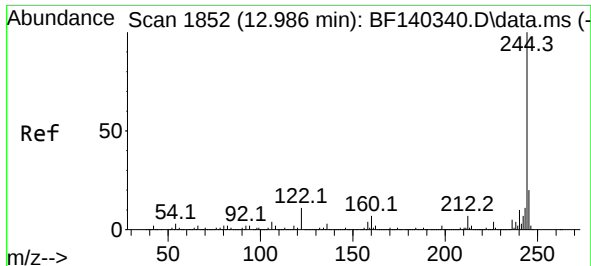


#79
 Terphenyl-d14
 Concen: 46.880 ng
 RT: 12.980 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF140507.D
 Acq: 20 Nov 2024 18:43


Instrument :
 BNA_F
 ClientSampleId :

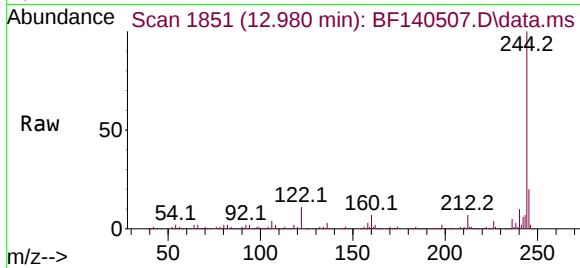

Tgt Ion:244 Resp: 546390
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.8 8.8
 122 10.6 8.8 13.2

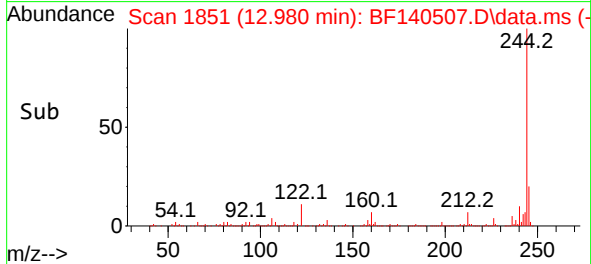

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2285
 Delta R.T. -0.024 min
 Lab File: BF140507.D
 Acq: 20 Nov 2024 18:43

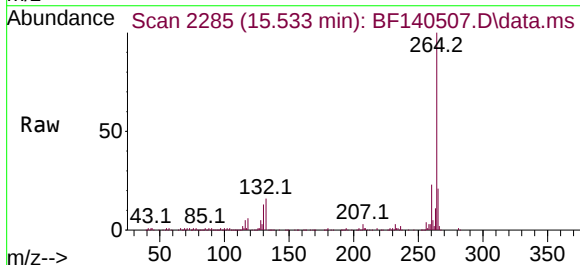

Tgt Ion:264 Resp: 204013
 Ion Ratio Lower Upper
 264 100
 260 23.0 19.2 28.8
 265 21.4 17.1 25.7

