
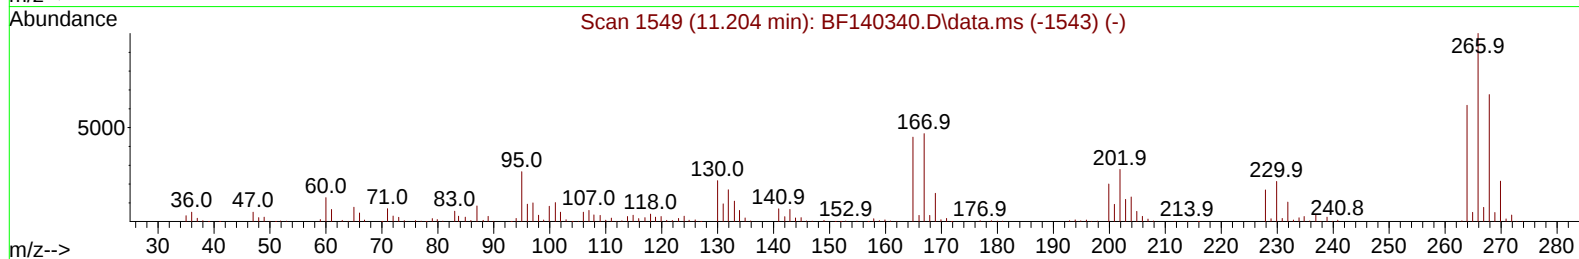
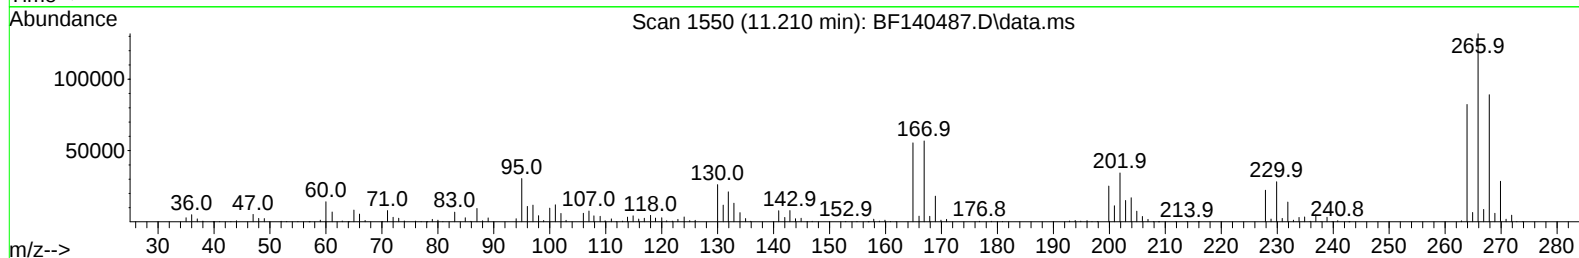


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140487.D
Acq On : 20 Nov 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 09:52:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

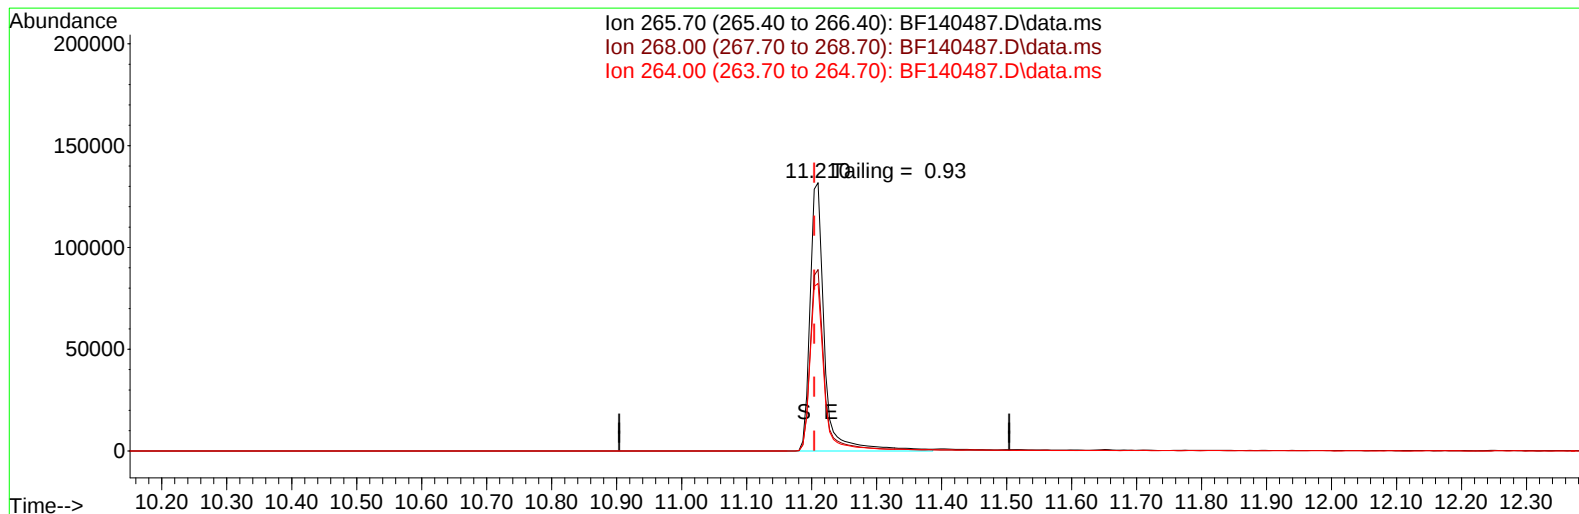

TIC: BF140487.D\data.ms

(70) Pentachlorophenol (C)




11.210min (+ 0.006) 71931.11 ng

response 204385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.61
264.00	62.90	62.46
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\  
Data File : BF140487.D  
Acq On    : 20 Nov 2024 09:04  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 20 09:52:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

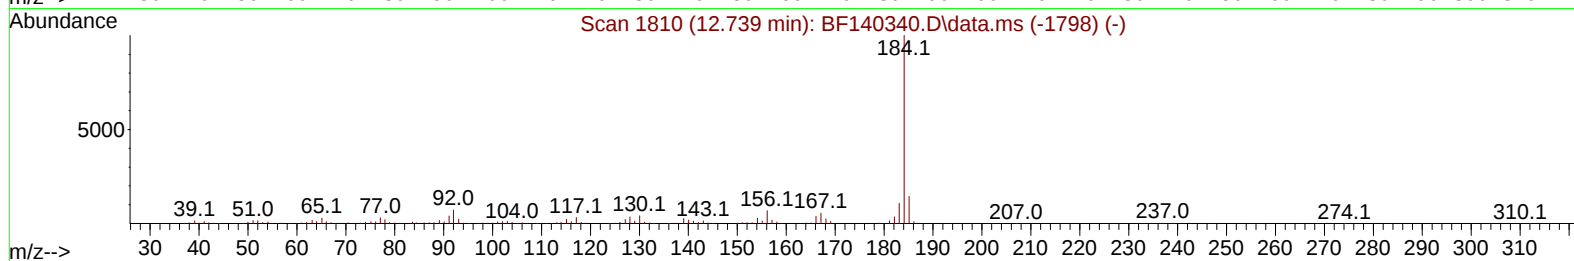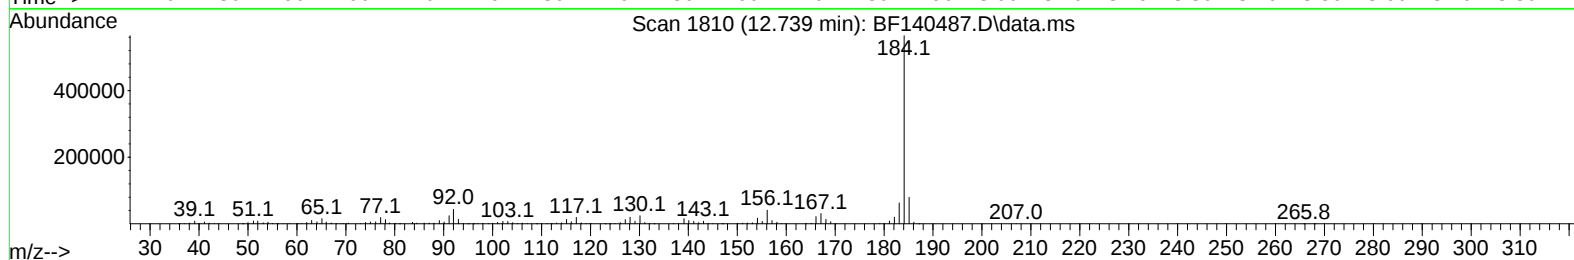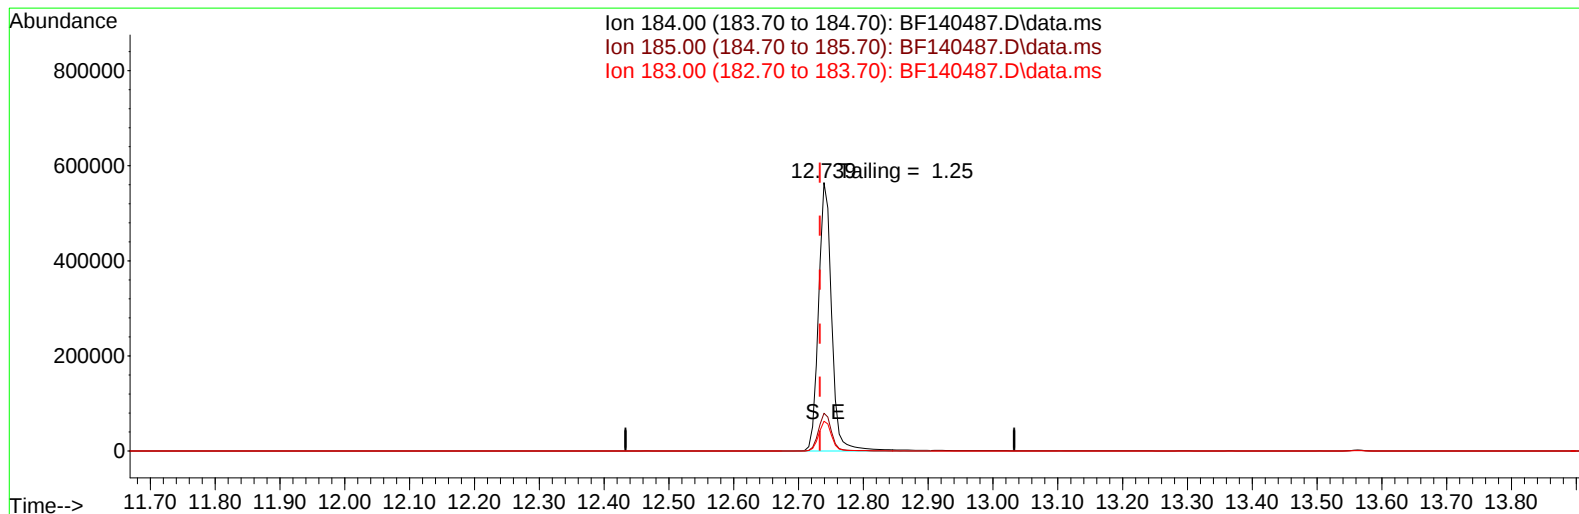

TIC: BF140487.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 26914.53 ng

response **799539**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.11
--------	-------	-------

183.00	10.80	11.08
--------	-------	-------

0.00 0.00 0.00