

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140498.D
Acq On : 20 Nov 2024 14:01
Operator : RC/JU
Sample : P4868-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW5-SP303-20241114RE

Quant Time: Nov 20 14:29:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.869	152	107774	20.000	ng	-0.01
21) Naphthalene-d8	8.151	136	401651	20.000	ng	0.00
39) Acenaphthene-d10	9.904	164	185909	20.000	ng	-0.01
64) Phenanthrene-d10	11.398	188	383896	20.000	ng	0.00
76) Chrysene-d12	14.039	240	211068	20.000	ng	-0.01
86) Perylene-d12	15.533	264	81264	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	415318	65.796	ng	0.00
7) Phenol-d6	6.504	99	315680	36.913	ng	0.00
23) Nitrobenzene-d5	7.434	82	813534	105.533	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	327454	177.125	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1392379	120.398	ng	0.00
79) Terphenyl-d14	12.986	244	1457190	119.837	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140498.D
Acq On : 20 Nov 2024 14:01
Operator : RC/JU
Sample : P4868-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW5-SP303-20241114RE

Quant Time: Nov 20 14:29:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration




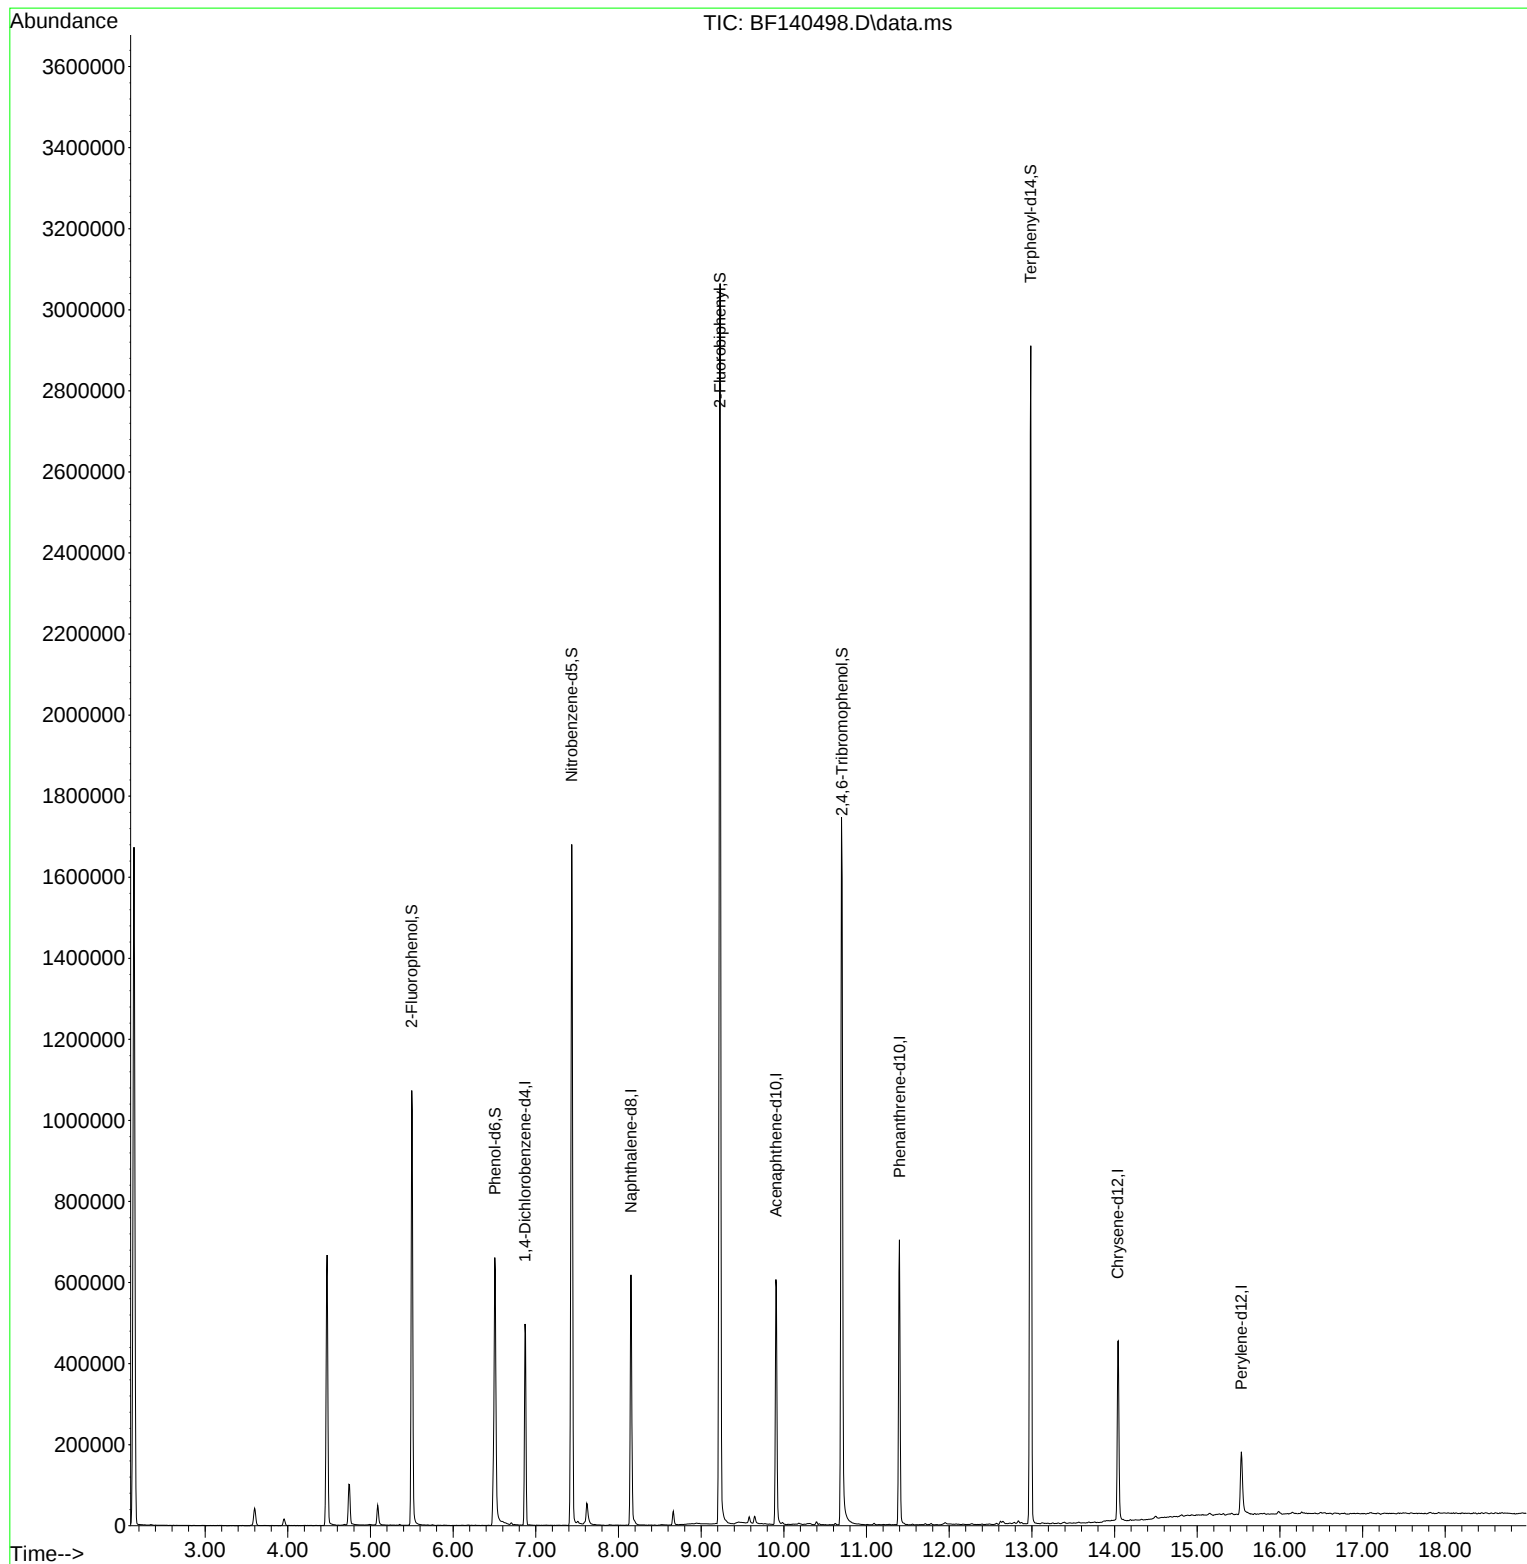


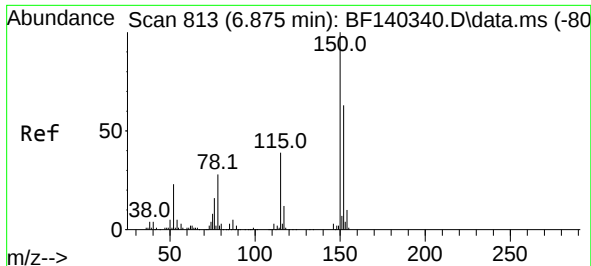

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.869 min Scan# 813
Delta R.T. -0.012 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01




Instrument :
BNA_F
ClientSampleId :
RW5-SP303-20241114RE

Tgt Ion:152 Resp: 107774
Ion Ratio Lower Upper
152 100
150 155.0 127.4 191.0
115 61.1 47.4 71.2

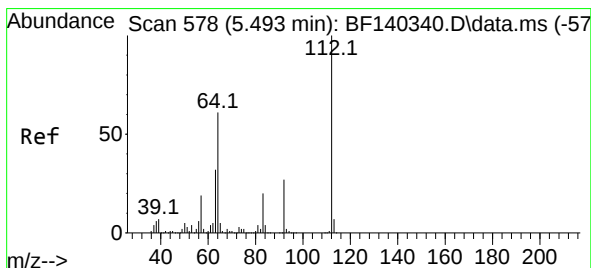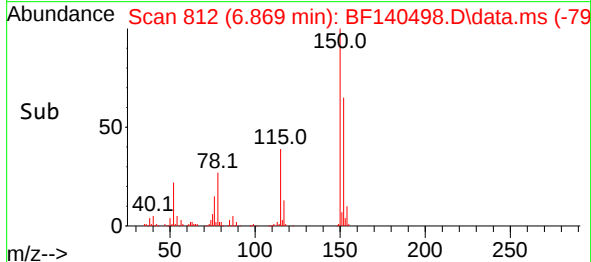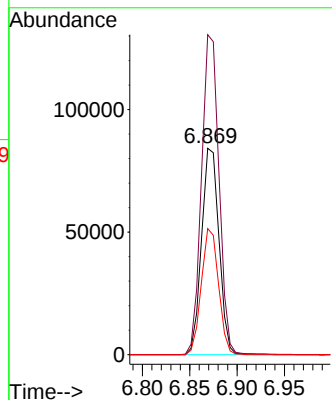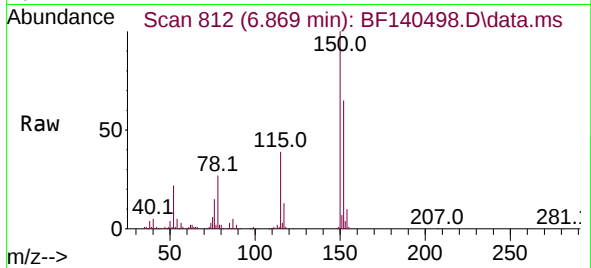

#5
2-Fluorophenol
Concen: 65.796 ng
RT: 5.498 min Scan# 579
Delta R.T. 0.006 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01

Tgt Ion:112 Resp: 415318
Ion Ratio Lower Upper
112 100
64 61.2 49.2 73.8
63 31.8 25.6 38.4


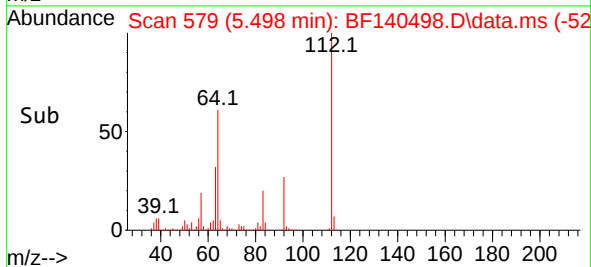
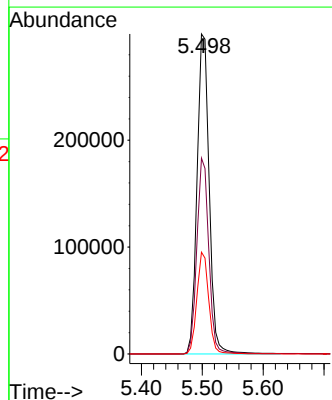
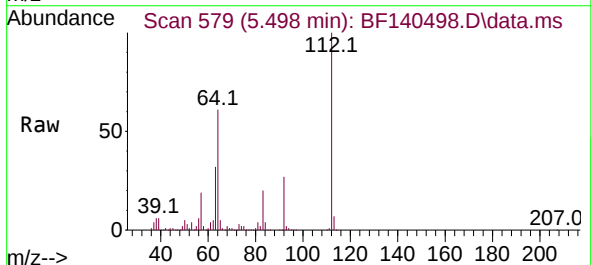




#7
Phenol-d6
Concen: 36.913 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01




Instrument :
BNA_F
ClientSampleId :
RW5-SP303-20241114RE


Tgt Ion: 99 Resp: 315680
Ion Ratio Lower Upper
99 100
42 18.5 15.1 22.7
71 34.6 27.9 41.9

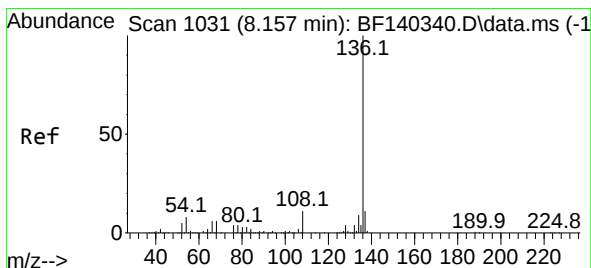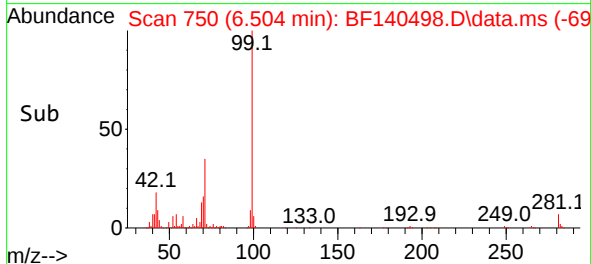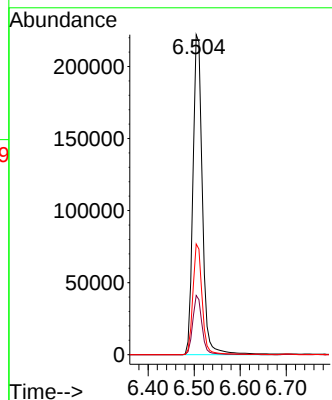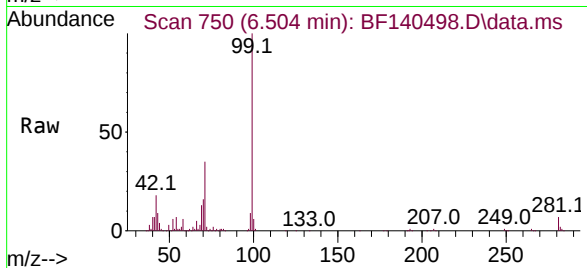

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.006 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01

Tgt Ion: 136 Resp: 401651
Ion Ratio Lower Upper
136 100
137 10.7 8.7 13.1
54 7.8 6.5 9.7
68 6.0 5.0 7.6

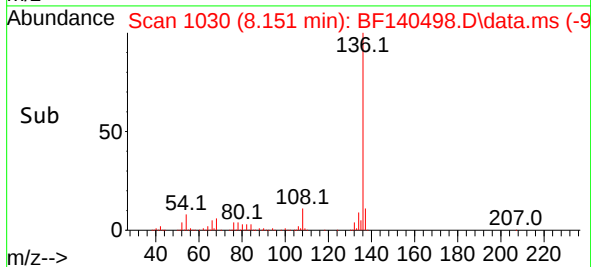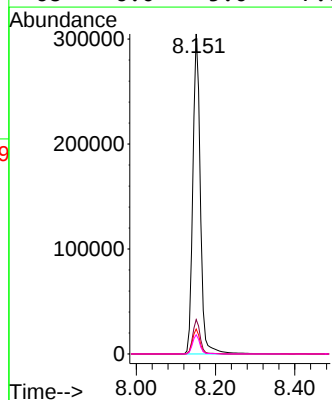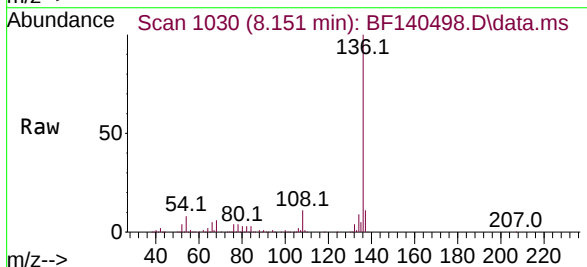

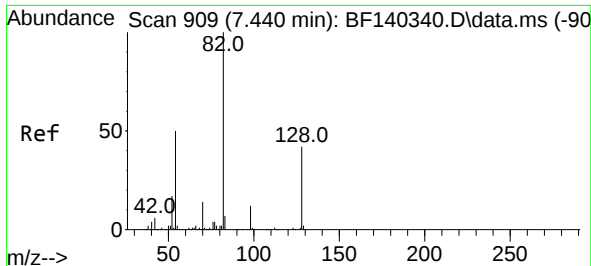

#23

Nitrobenzene-d5

Concen: 105.533 ng

RT: 7.434 min Scan# 90

Delta R.T. -0.006 min

Lab File: BF140498.D

Acq: 20 Nov 2024 14:01

Instrument :





BNA_F

ClientSampleId :

RW5-SP303-20241114RE

Tgt Ion: 82 Resp: 813534

Ion	Ratio	Lower	Upper
82	100		
128	42.6	33.3	49.9
54	48.6	39.8	59.8

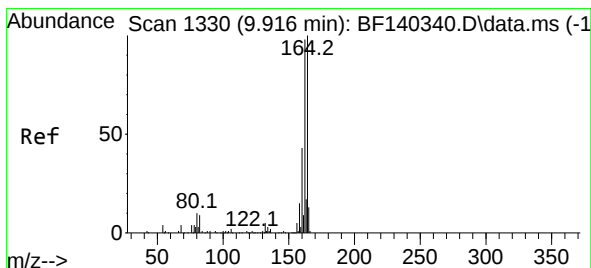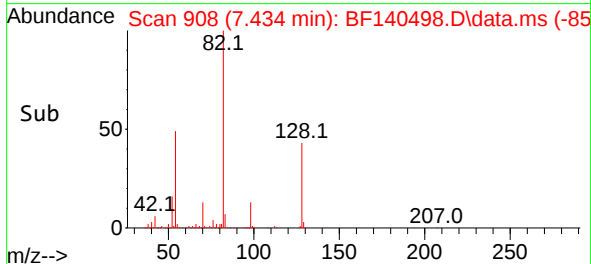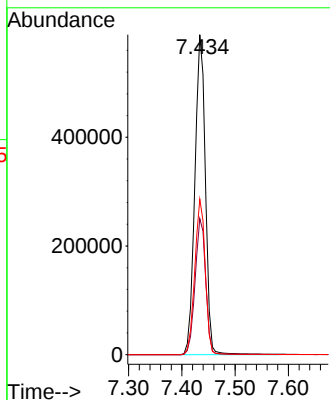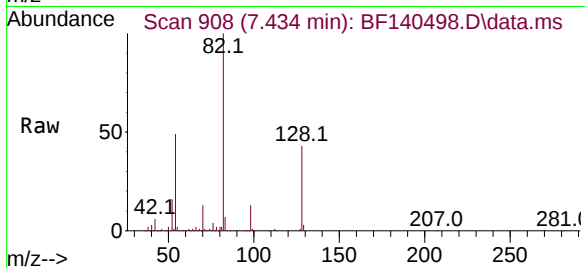

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.904 min Scan# 1328




Delta R.T. -0.012 min

Lab File: BF140498.D

Acq: 20 Nov 2024 14:01

Tgt Ion: 164 Resp: 185909

Ion	Ratio	Lower	Upper
164	100		
162	101.0	79.8	119.8
160	45.3	35.4	53.0

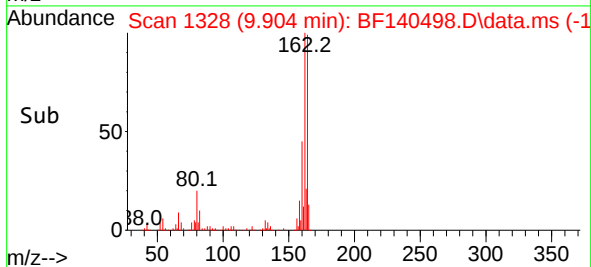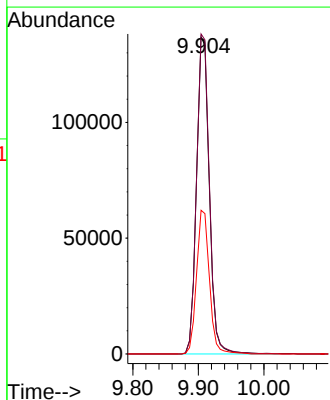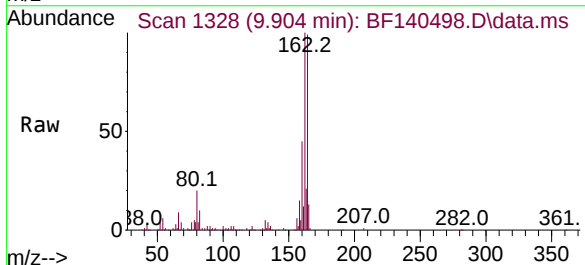



#42

2,4,6-Tribromophenol

Concen: 177.125 ng

RT: 10.704 min Scan# 1464

Delta R.T. -0.000 min

Lab File: BF140498.D

Acq: 20 Nov 2024 14:01

Instrument :

BNA_F

ClientSampleId :

RW5-SP303-20241114RE





Tgt Ion:330 Resp: 327454

Ion Ratio Lower Upper

330 100

332 96.7 75.9 113.9

141 32.5 26.9 40.3

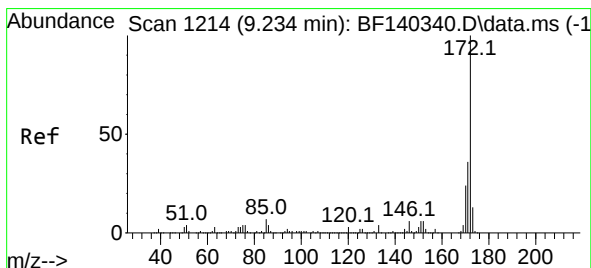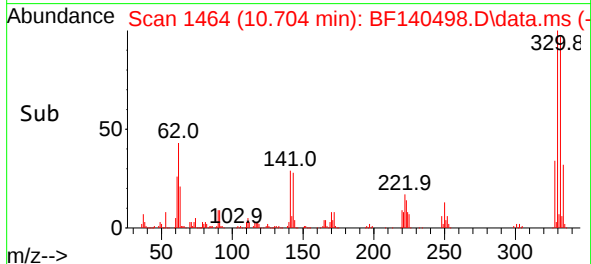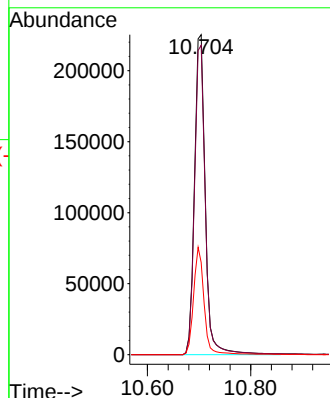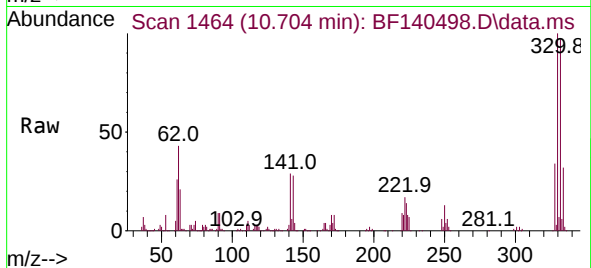

#45

2-Fluorobiphenyl

Concen: 120.398 ng

RT: 9.228 min Scan# 1213

Delta R.T. -0.006 min

Lab File: BF140498.D

Acq: 20 Nov 2024 14:01




Tgt Ion:172 Resp: 1392379


Ion Ratio Lower Upper

172 100

171 35.8 28.5 42.7

170 23.6 19.1 28.7


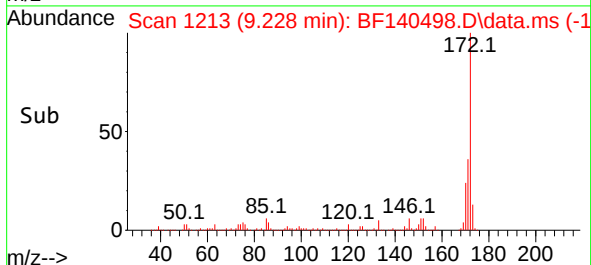
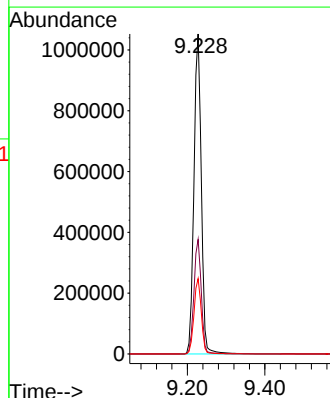
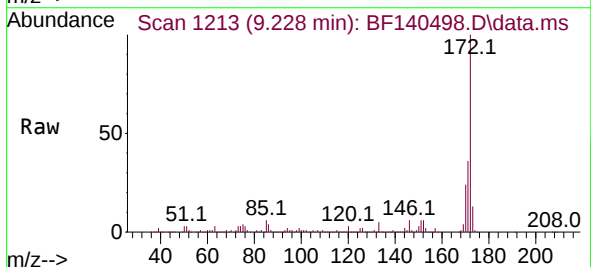


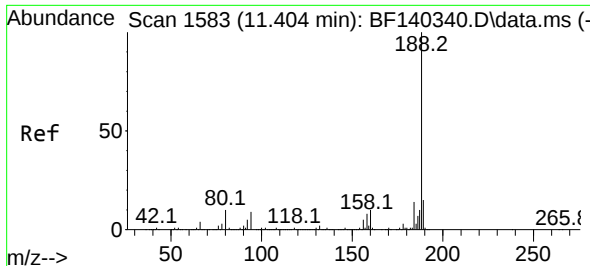

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01




Instrument :
BNA_F
ClientSampleId :
RW5-SP303-20241114RE


Tgt Ion:188 Resp: 383896
Ion Ratio Lower Upper
188 100
94 9.0 7.6 11.4
80 9.9 8.0 12.0

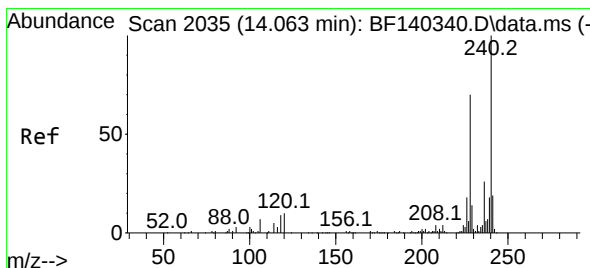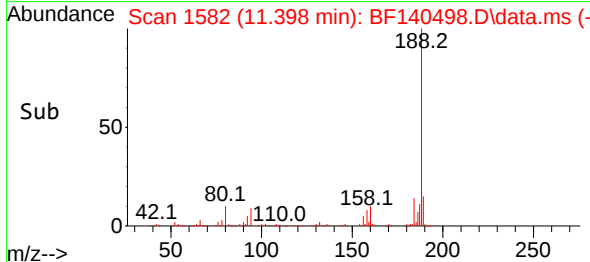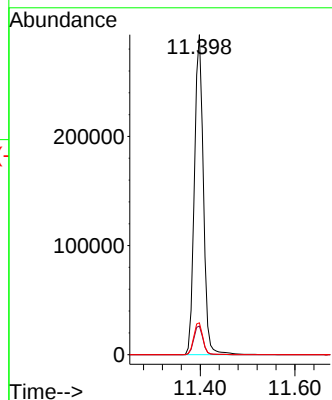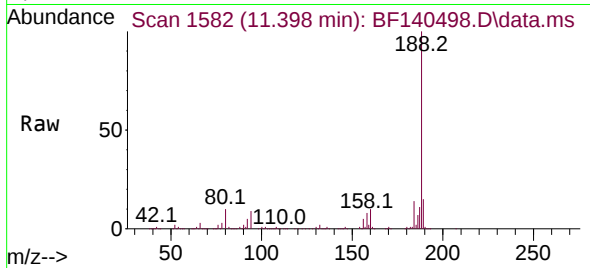

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2031
Delta R.T. -0.012 min
Lab File: BF140498.D
Acq: 20 Nov 2024 14:01


Tgt Ion:240 Resp: 211068
Ion Ratio Lower Upper
240 100
120 11.4 8.8 13.2
236 27.0 20.9 31.3

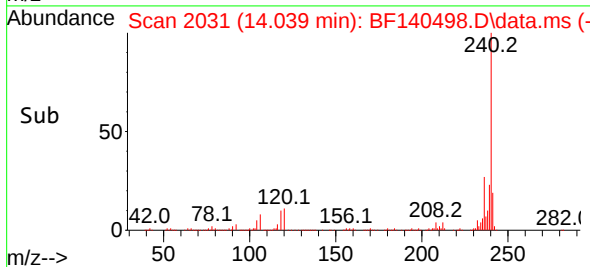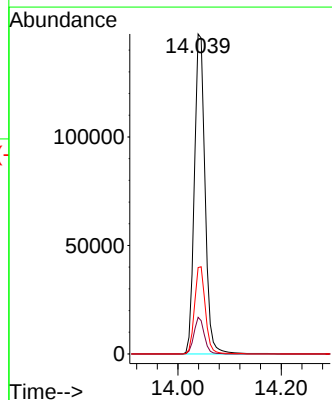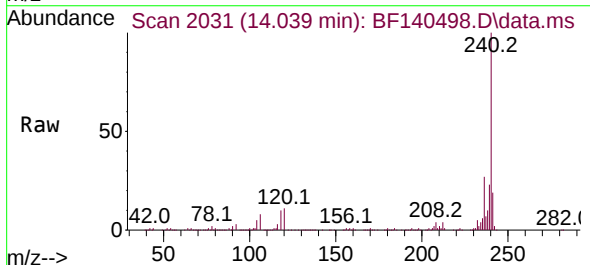



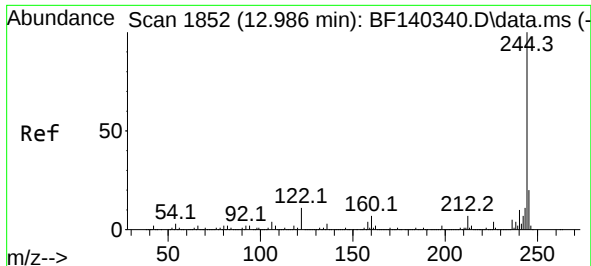


#79
 Terphenyl-d14
 Concen: 119.837 ng
 RT: 12.986 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF140498.D
 Acq: 20 Nov 2024 14:01


Instrument :
 BNA_F
 ClientSampleId :
 RW5-SP303-20241114RE

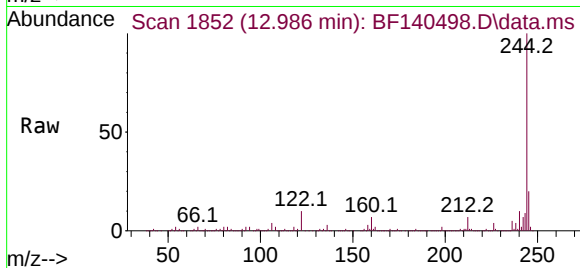

Tgt Ion:244 Resp: 1457190
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.8
 122 10.4 8.8 13.2

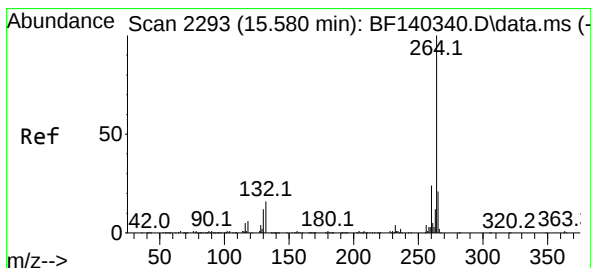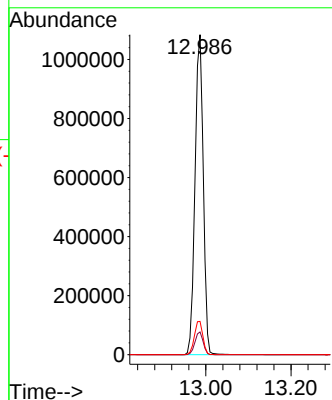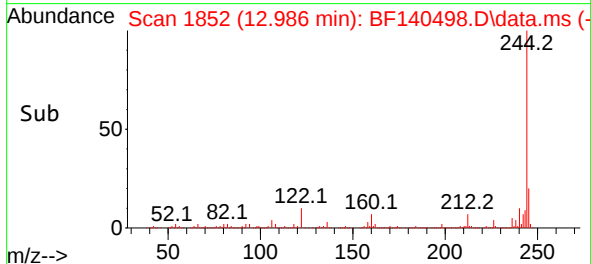

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2285
 Delta R.T. -0.024 min
 Lab File: BF140498.D
 Acq: 20 Nov 2024 14:01

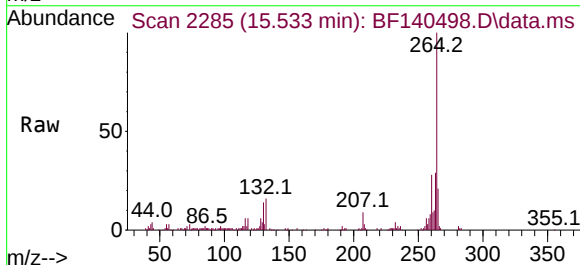

Tgt Ion:264 Resp: 81264
 Ion Ratio Lower Upper
 264 100
 260 28.1 19.2 28.8
 265 21.1 17.1 25.7

