


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140487.D
Acq On : 20 Nov 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

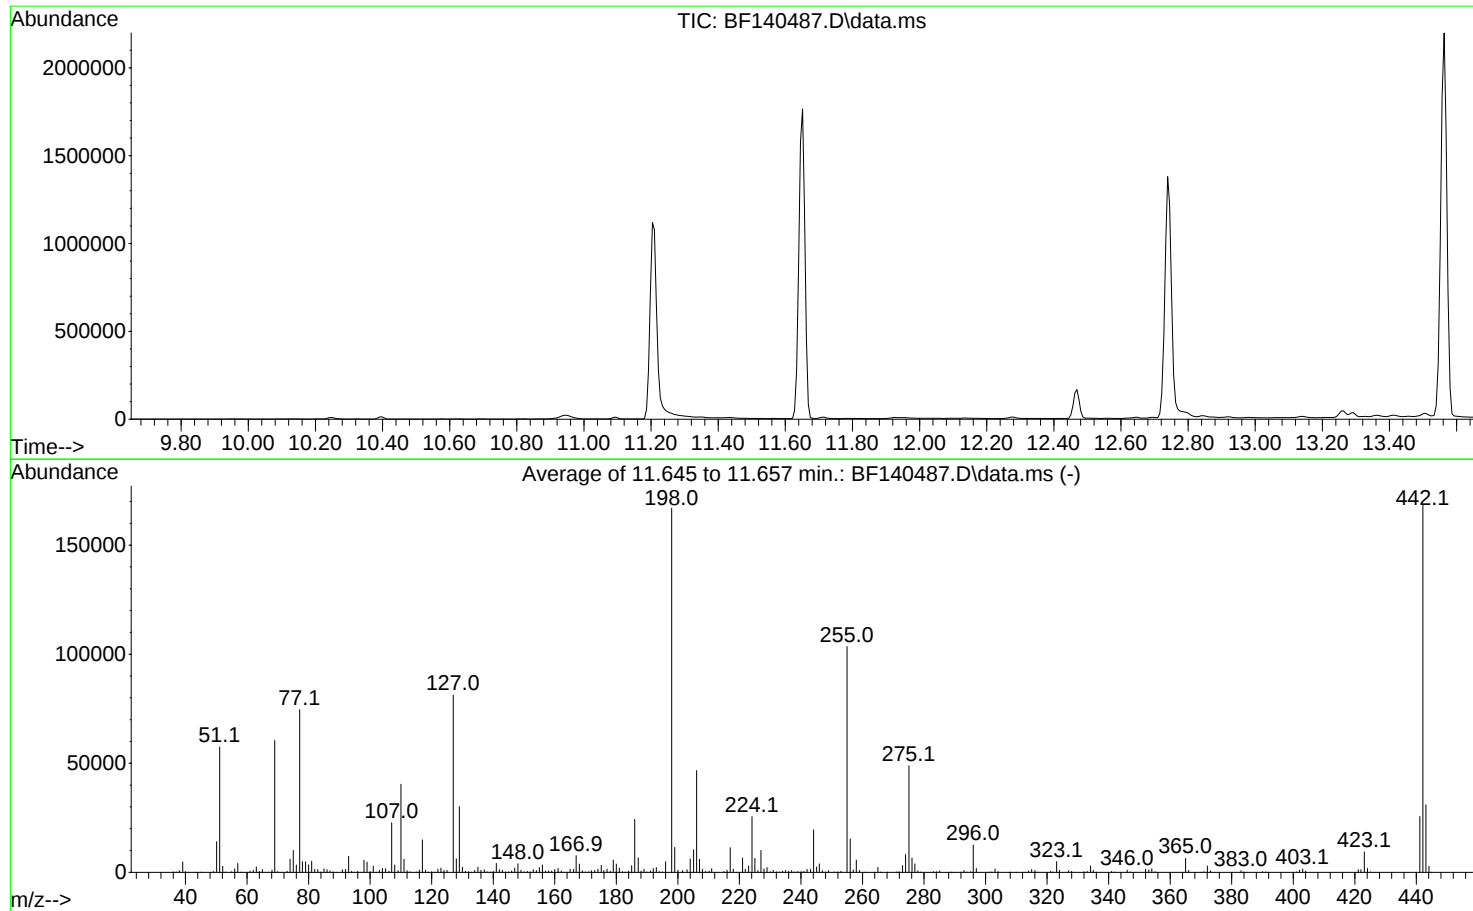

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	34.4	57483	PASS
68	69	0.00	2	1.9	1125	PASS
69	198	0.00	100	36.2	60485	PASS
70	69	0.00	2	0.6	336	PASS
127	198	10	80	48.7	81299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	166936	PASS
199	198	5	9	6.8	11421	PASS
275	198	10	60	29.3	48829	PASS
365	198	1	100	3.8	6418	PASS
441	198	0.01	100	15.3	25587	PASS
442	442	50	100	100.0	168640	PASS
443	442	15	24	18.3	30941	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/20/2024	BNA_F	<u>BF140487.D</u>
Compound Name	Response	Retention Time
DDT	548781	13.563
DDD	16051	13.263
DDE	1359	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17410	566191	3.07

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140487.D
Acq On : 20 Nov 2024 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 20 09:52:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

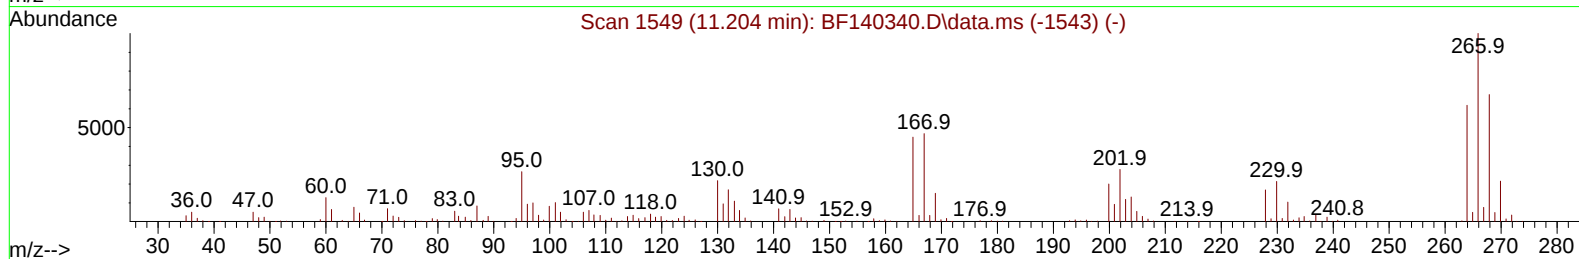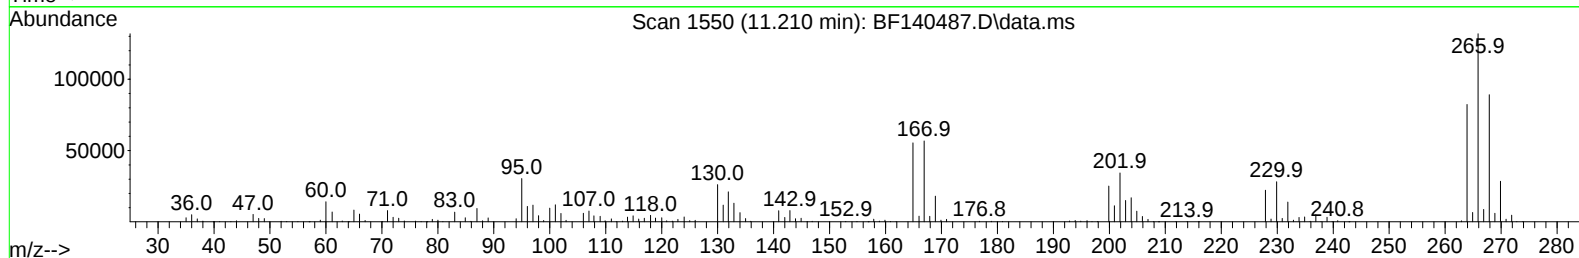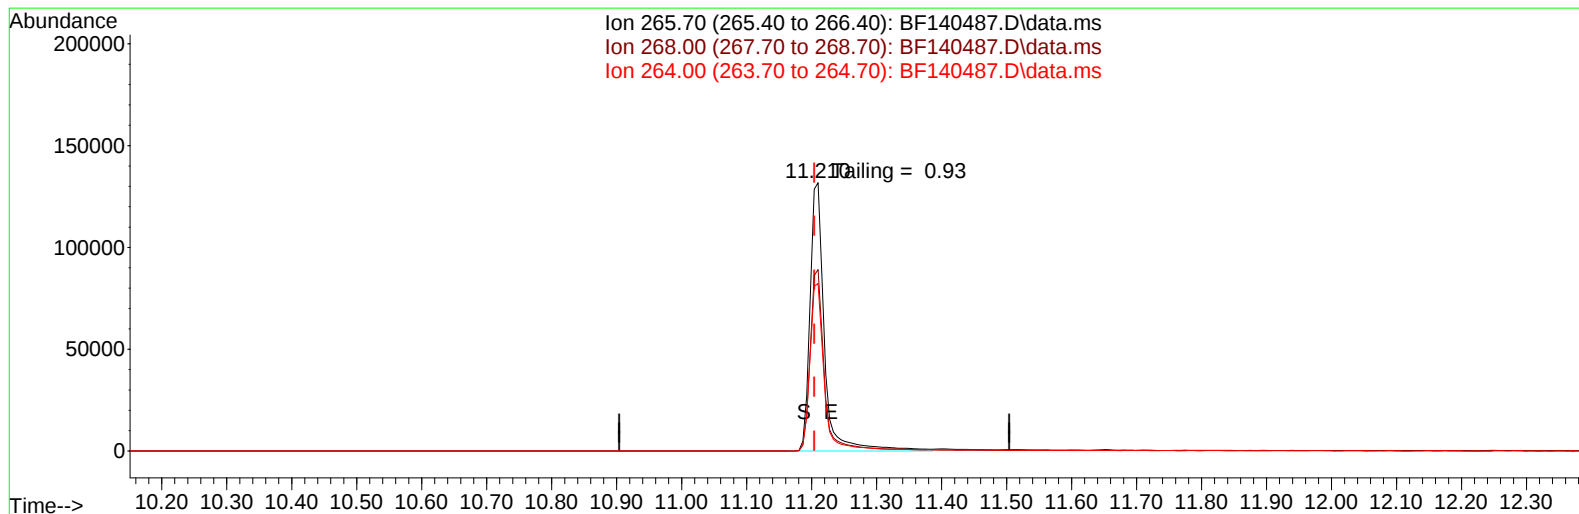

TIC: BF140487.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.006) 71931.11 ng

response 204385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.61
264.00	62.90	62.46
0.00	0.00	0.00

