

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
 Data File : BF144293.D
 Acq On : 20 Nov 2025 14:24
 Operator : RC/JU
 Sample : PB170652BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB170652BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	486	493	507	rBV	307671	503926	25.51%	4.026%
2	5.492	555	561	581	rBV	1157961	1569575	79.45%	12.539%
3	6.492	725	731	748	rBV	1112045	1592696	80.62%	12.723%
4	6.863	789	794	801	rBV	279150	343953	17.41%	2.748%
5	7.422	884	889	903	rBV	731630	1014756	51.37%	8.107%
6	8.145	1006	1012	1025	rBV	346127	453349	22.95%	3.622%
7	9.222	1189	1195	1200	rBV	1487720	1975511	100.00%	15.782%
8	9.898	1305	1310	1322	rBV	425995	549683	27.82%	4.391%
9	10.692	1440	1445	1464	rBV	1012033	1313828	66.51%	10.496%
10	11.392	1558	1564	1571	rBV	422385	542067	27.44%	4.330%
11	12.980	1828	1834	1839	rBV	1392730	1811197	91.68%	14.469%
12	13.874	1965	1986	2000	rBV5	11790	60584	3.07%	0.484%
13	14.039	2009	2014	2026	rBV	273085	354486	17.94%	2.832%
14	15.515	2259	2265	2274	rBV	257258	411307	20.82%	3.286%
15	16.480	2424	2429	2438	rVB4	9846	20835	1.05%	0.166%




Sum of corrected areas: 12517753

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144293.D
Acq On : 20 Nov 2025 14:24
Operator : RC/JU
Sample : PB170652BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170652BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

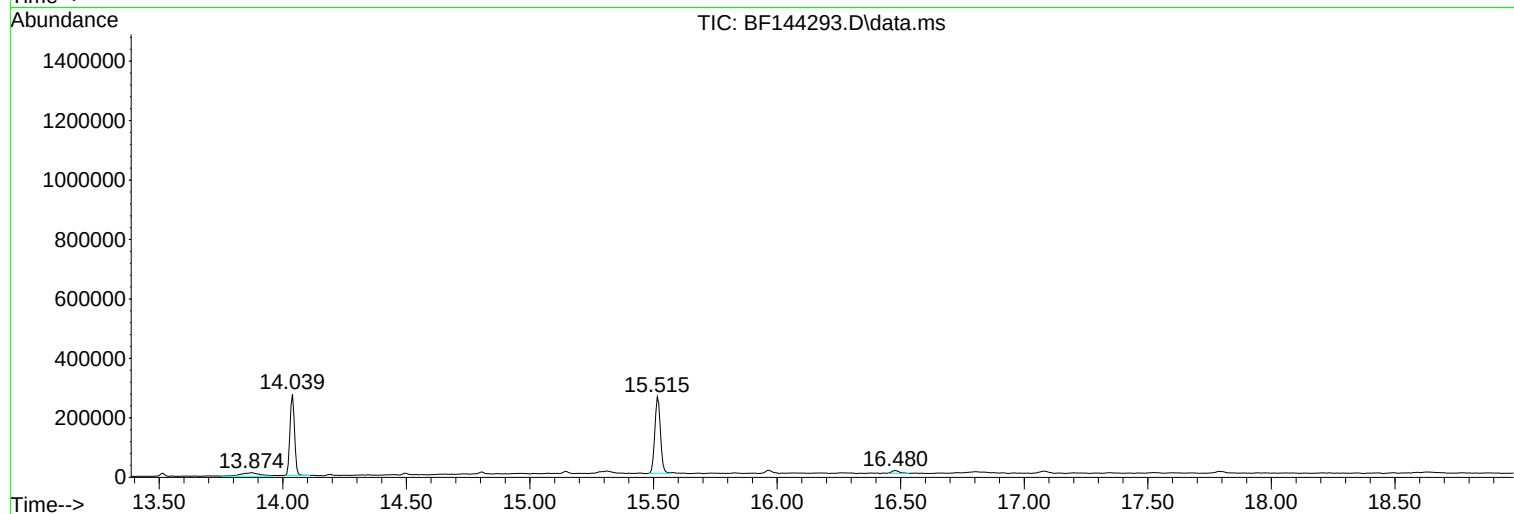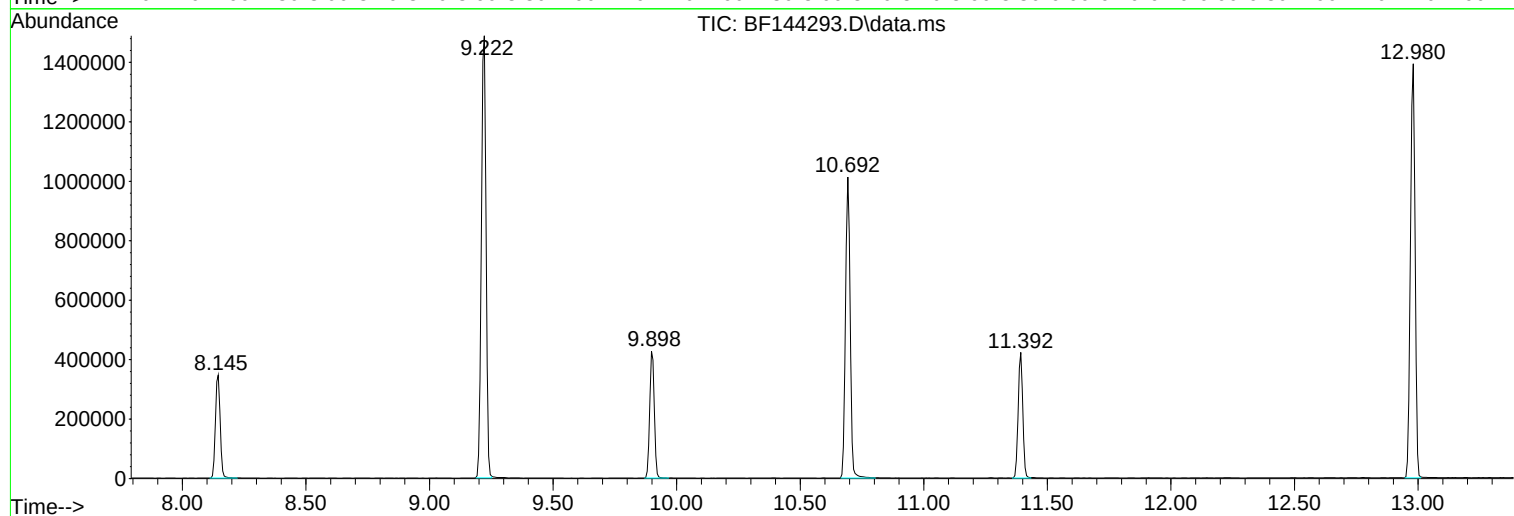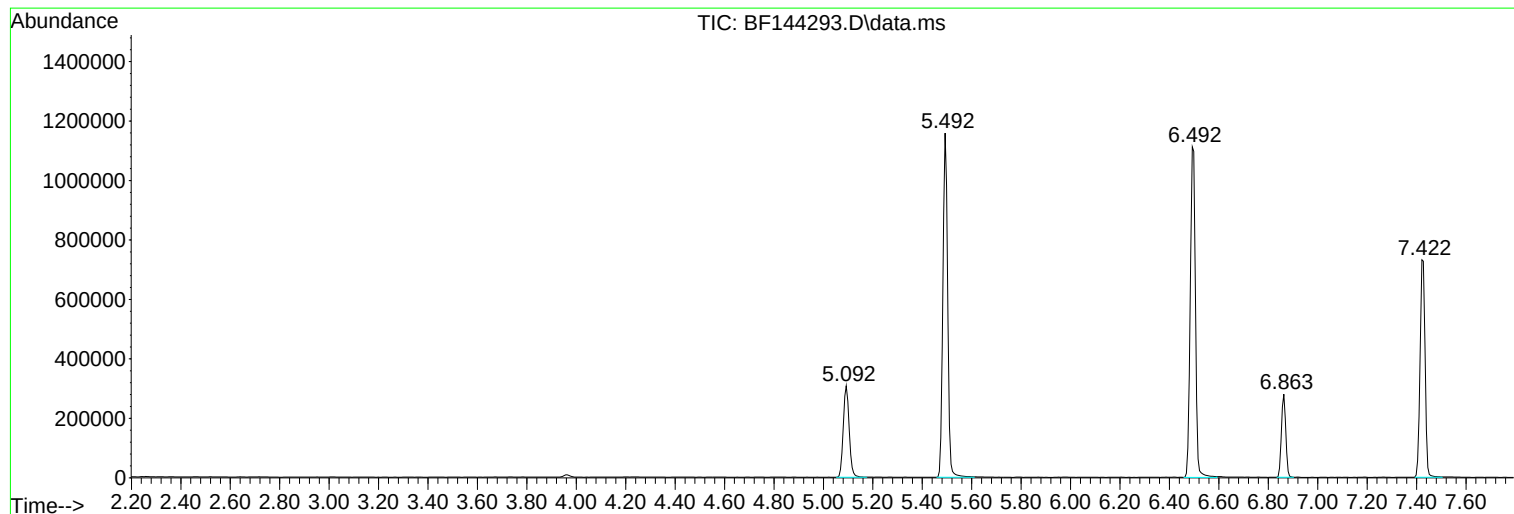

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144293.D
Acq On : 20 Nov 2025 14:24
Operator : RC/JU
Sample : PB170652BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170652BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144293.D
Acq On : 20 Nov 2025 14:24
Operator : RC/JU
Sample : PB170652BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170652BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------