


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144289.D
Acq On : 20 Nov 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

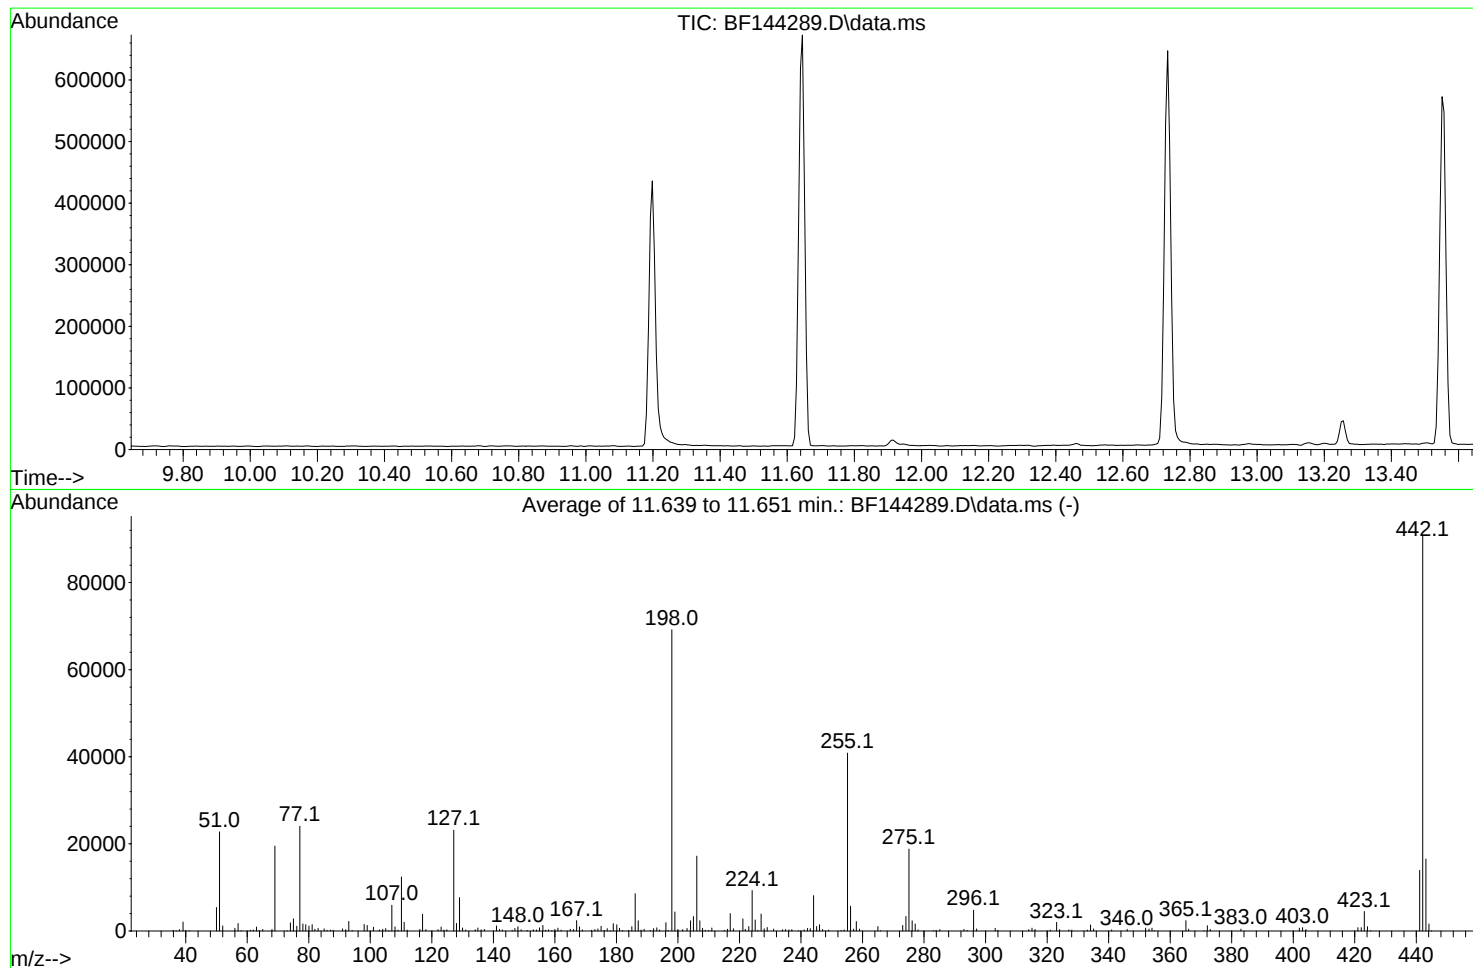




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1599

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	346	PASS
69	69	100	100	100.0	19512	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	69195	PASS
199	198	5	9	6.3	4369	PASS
365	198	1	100	3.4	2362	PASS
441	443	0.01	150	84.3	13903	PASS
442	442	100	100	100.0	90677	PASS
443	442	15	24	18.2	16500	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144289.D
Acq On : 20 Nov 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 20 12:22:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

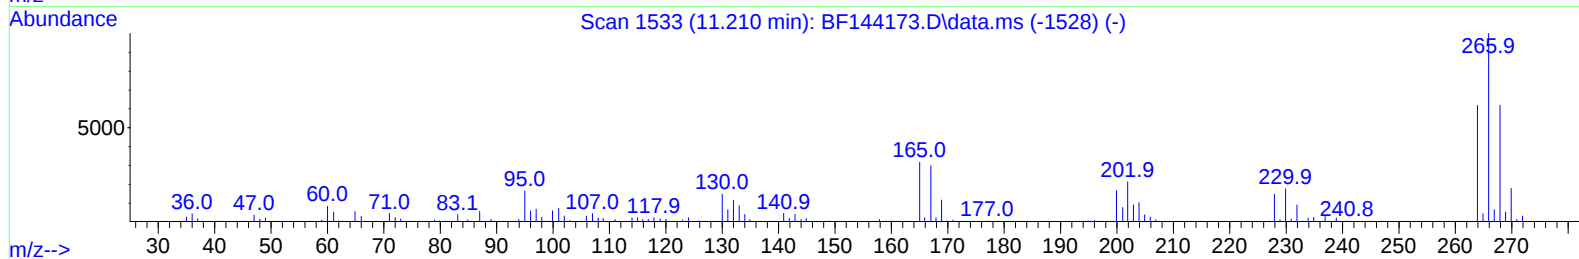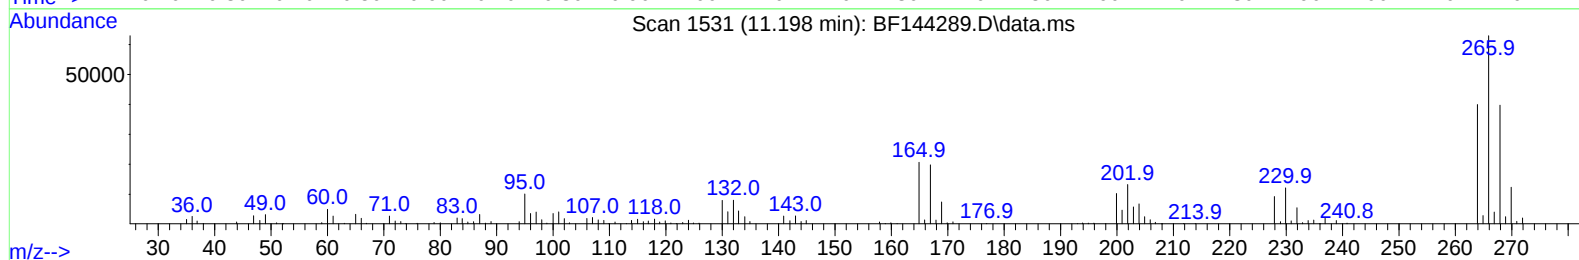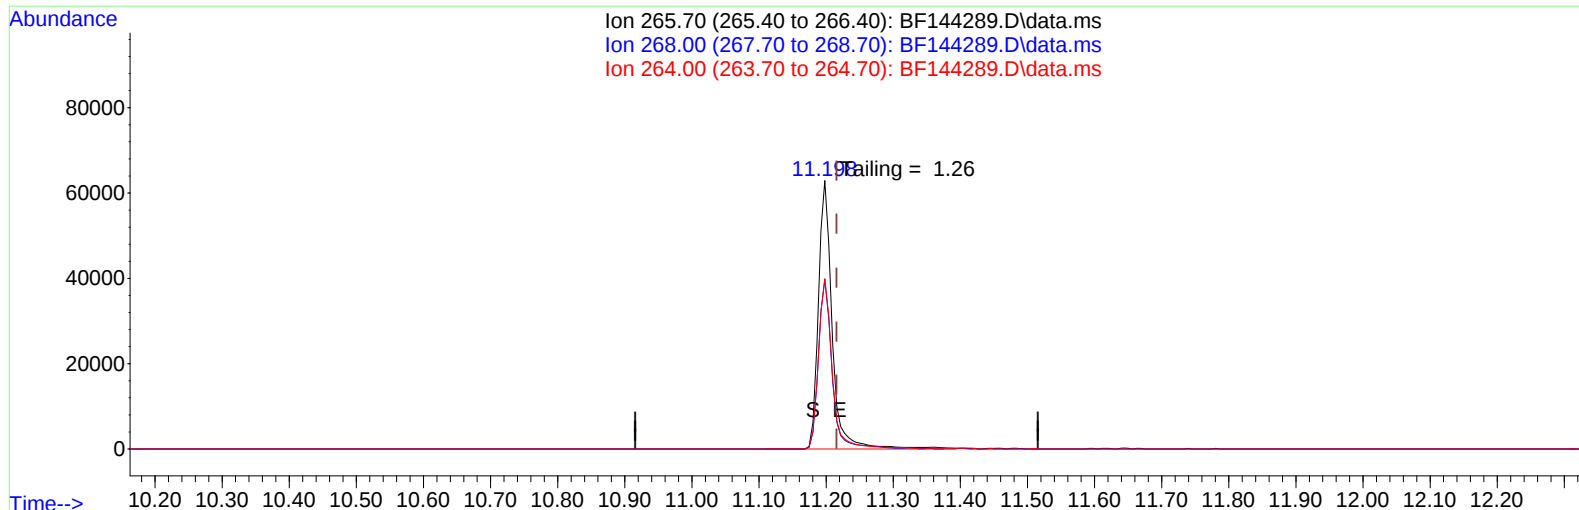

TIC: BF144289.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 59695.02 ng




response 88935

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.17
264.00	61.80	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112025\
Data File : BF144289.D
Acq On : 20 Nov 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 20 12:22:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

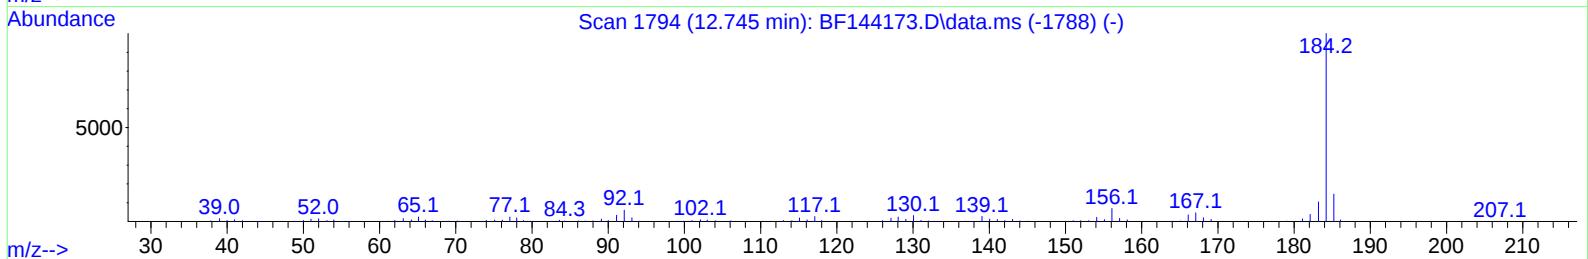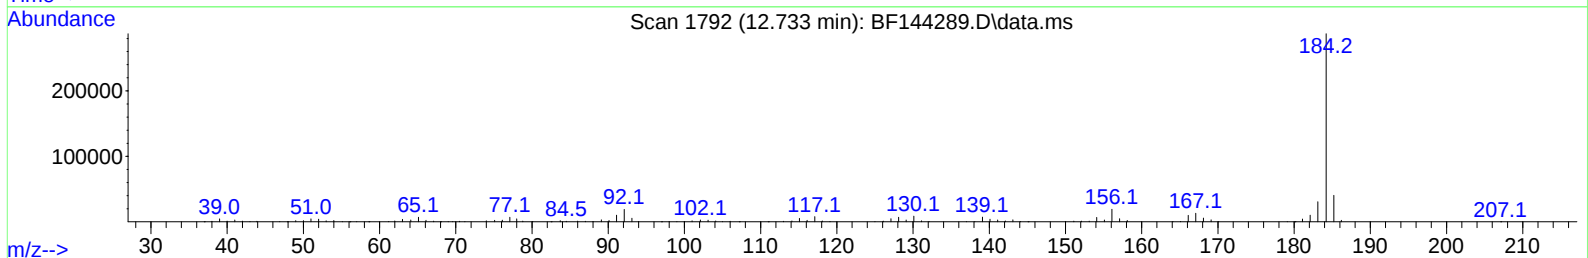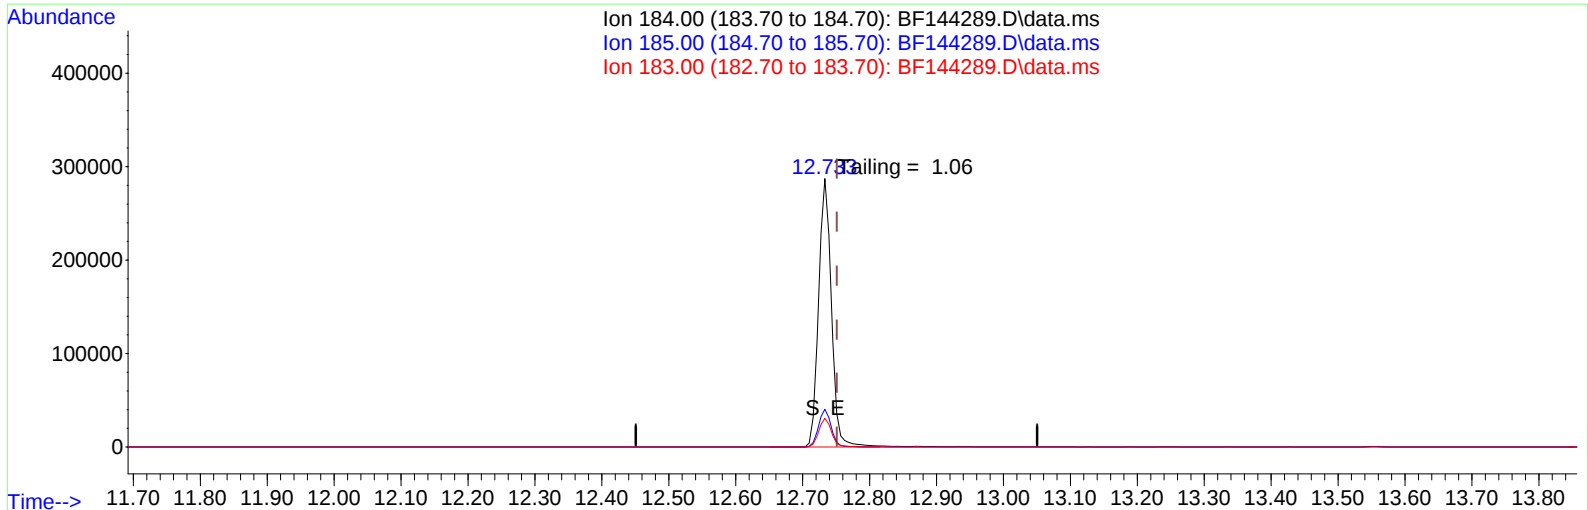

TIC: BF144289.D\data.ms

(77) Benzidine

12.733min (-0.018) 0.00 ng

response 383431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.07
183.00	10.40	10.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/20/2025	BNA_F	<u>BF144289.D</u>
Compound Name	Response	Retention Time
DDT	159048	13.551
DDD		13.257
DDE	56	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56	159104	0.04

Instrument :
BNA_F
ClientSampleId :
DFTPP