

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112118\
 Data File : BF110922.D
 Acq On : 21 Nov 2018 12:25
 Operator : JU/SJ
 Sample : J5957-02RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-2RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.205	15	20	47	rVB	243884	382230	57.72%	3.555%
2	5.169	522	524	530	rBV2	6347	11048	1.67%	0.103%
3	5.569	589	592	609	rBV	95083	187219	28.27%	1.741%
4	6.581	759	764	783	rBV2	158112	336927	50.88%	3.133%
5	6.710	783	786	796	rVV	454933	429537	64.87%	3.994%
6	6.940	822	825	832	rBV	391139	350118	52.87%	3.256%
7	7.093	848	851	866	rBV	367856	400320	60.45%	3.723%
8	7.510	918	922	944	rBV	214801	325844	49.21%	3.030%
9	7.657	944	947	949	rVB	22442	18803	2.84%	0.175%
10	8.222	1040	1043	1065	rBV	401725	484180	73.12%	4.503%
11	9.292	1222	1225	1235	rBV	574154	605713	91.47%	5.633%
12	9.692	1290	1293	1304	rVB	61840	74386	11.23%	0.692%
13	9.981	1339	1342	1353	rBV	522871	547577	82.69%	5.092%
14	10.386	1409	1411	1415	rVB	11565	8240	1.24%	0.077%
15	10.781	1474	1478	1489	rBV	280628	331078	50.00%	3.079%
16	10.869	1489	1493	1497	rVB2	10655	15287	2.31%	0.142%
17	11.480	1593	1597	1608	rBV	596707	603654	91.16%	5.614%
18	11.980	1677	1682	1698	rBV	279636	373517	56.41%	3.473%
19	12.322	1737	1740	1742	rVB4	11897	10975	1.66%	0.102%
20	12.627	1790	1792	1797	rBV5	6231	7820	1.18%	0.073%
21	12.680	1798	1801	1802	rBV3	7913	8359	1.26%	0.078%
22	12.704	1803	1805	1810	rVB2	8298	10940	1.65%	0.102%
23	12.769	1811	1816	1829	rBV	275055	378823	57.21%	3.523%
24	12.939	1842	1845	1851	rVB	17501	22492	3.40%	0.209%
25	13.057	1862	1865	1871	rVB	766257	662185	100.00%	6.158%
26	13.263	1896	1900	1905	rVB3	18154	22596	3.41%	0.210%
27	13.522	1941	1944	1949	rBV7	6087	9797	1.48%	0.091%
28	13.604	1954	1958	1961	rBV	34753	34596	5.22%	0.322%
29	13.933	2011	2014	2022	rBV	205748	274725	41.49%	2.555%
30	14.074	2036	2038	2042	rVB	10629	9172	1.39%	0.085%
31	14.133	2044	2048	2059	rBV	442889	510515	77.10%	4.747%
32	14.245	2064	2067	2071	rVV	119759	115991	17.52%	1.079%
33	14.551	2115	2119	2123	rBV	292410	266140	40.19%	2.475%
34	14.868	2169	2173	2179	rBV	449175	475813	71.85%	4.425%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112118\
Data File : BF110922.D
Acq On : 21 Nov 2018 12:25
Operator : JU/SJ
Sample : J5957-02RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-2RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.945	2183	2186	2191	rVB2	15470	15876	2.40%	0.148%
36	15.221	2227	2233	2243	rBV	489627	605418	91.43%	5.630%
37	15.610	2294	2299	2305	rBV	454093	610497	92.19%	5.677%
38	15.668	2305	2309	2322	rVB	205216	352690	53.26%	3.280%
39	15.886	2343	2346	2351	rVB4	13204	19886	3.00%	0.185%
40	16.063	2370	2376	2381	rBV	294555	451966	68.25%	4.203%
41	16.151	2385	2391	2392	rBV5	15605	27496	4.15%	0.256%
42	16.380	2428	2430	2435	rVB6	8474	9801	1.48%	0.091%
43	16.592	2459	2466	2474	rVB	121643	222080	33.54%	2.065%
44	17.209	2565	2571	2578	rVB2	37696	74448	11.24%	0.692%
45	17.933	2688	2694	2705	rBV6	16030	41429	6.26%	0.385%
46	18.392	2766	2772	2773	rBV5	8369	15164	2.29%	0.141%


Sum of corrected areas: 10753368

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112118\
Data File : BF110922.D
Acq On : 21 Nov 2018 12:25
Operator : JU/SJ
Sample : J5957-02RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
W-2RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

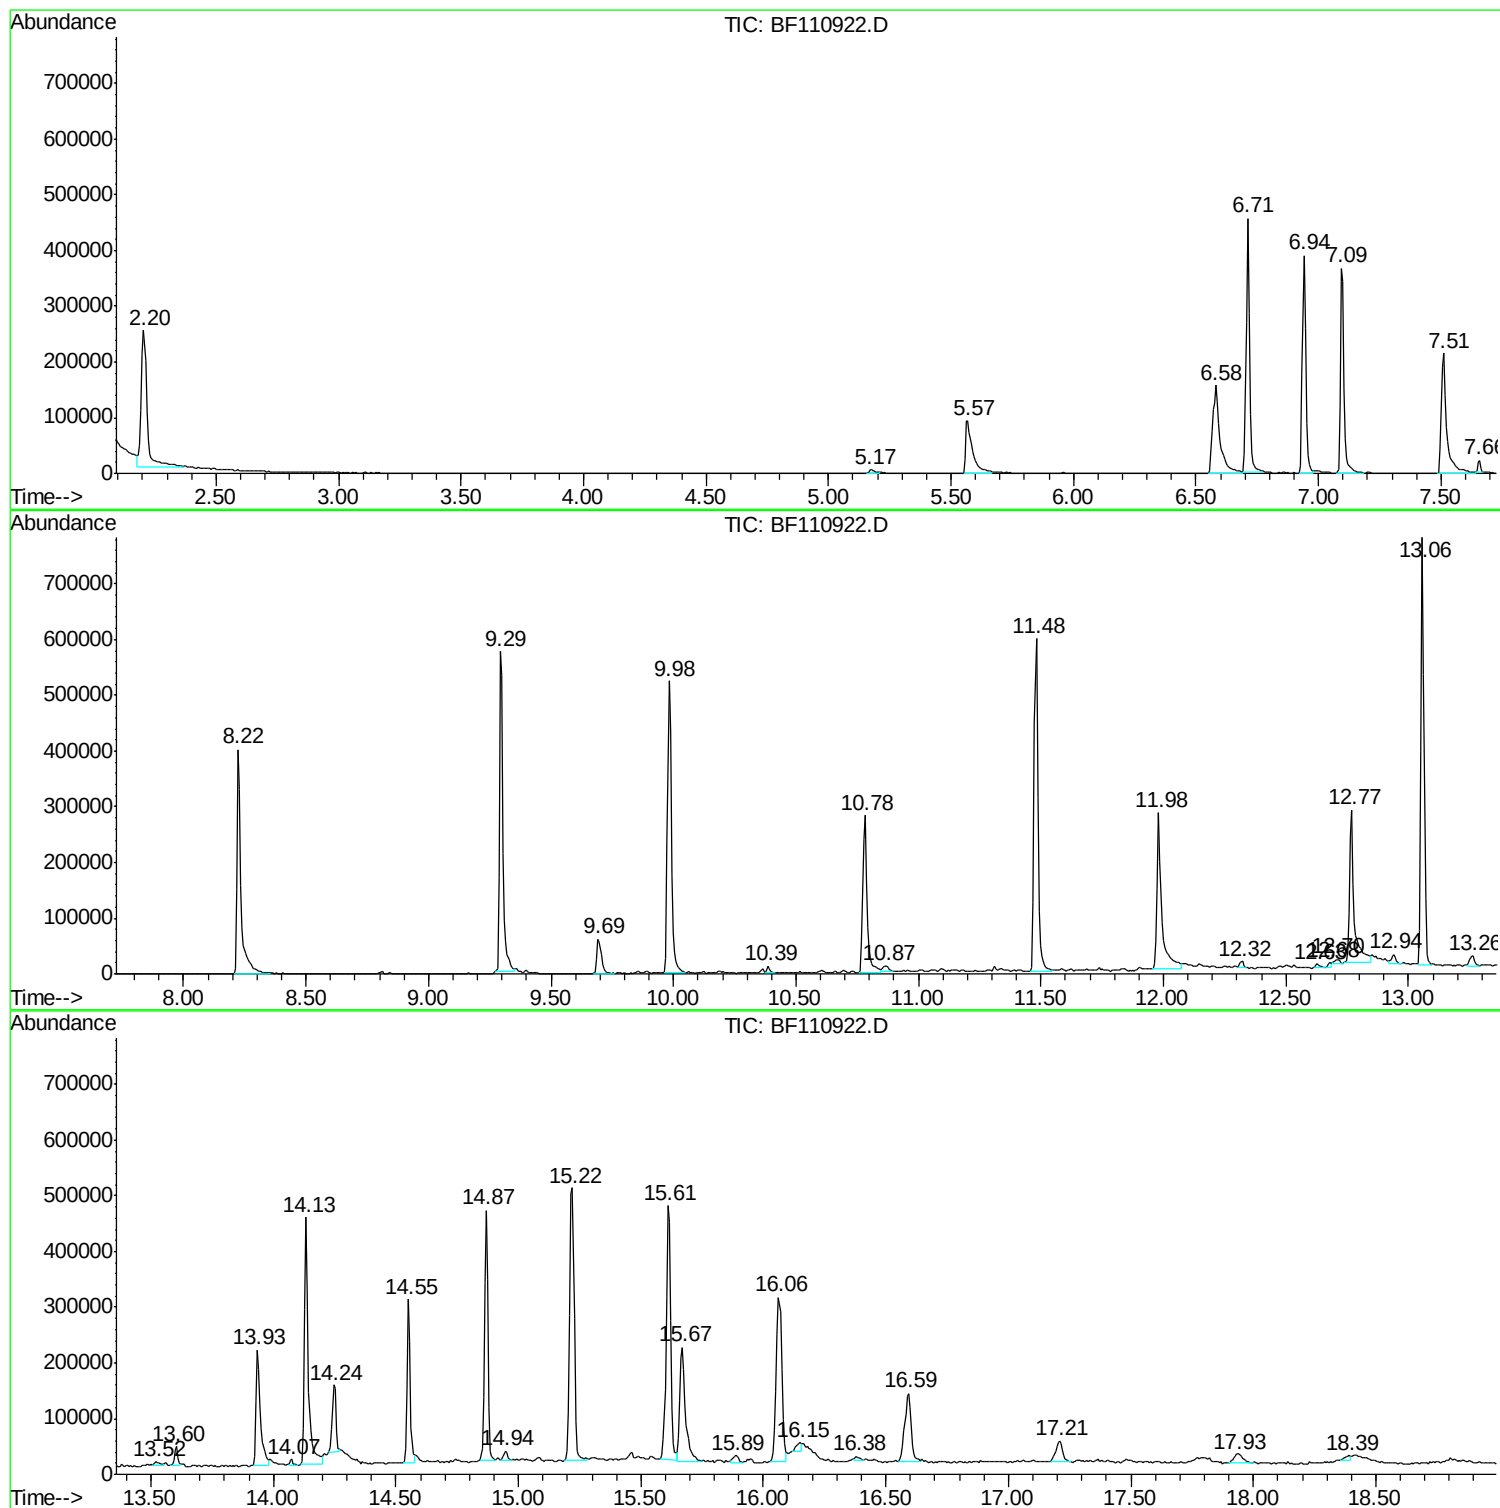

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112118\
Data_File : BF110922.D
Acq_On : 21-Nov-2018 12:255
Operator : JU/SJJ
Sample : J5957-02REE
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
W-2RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
