
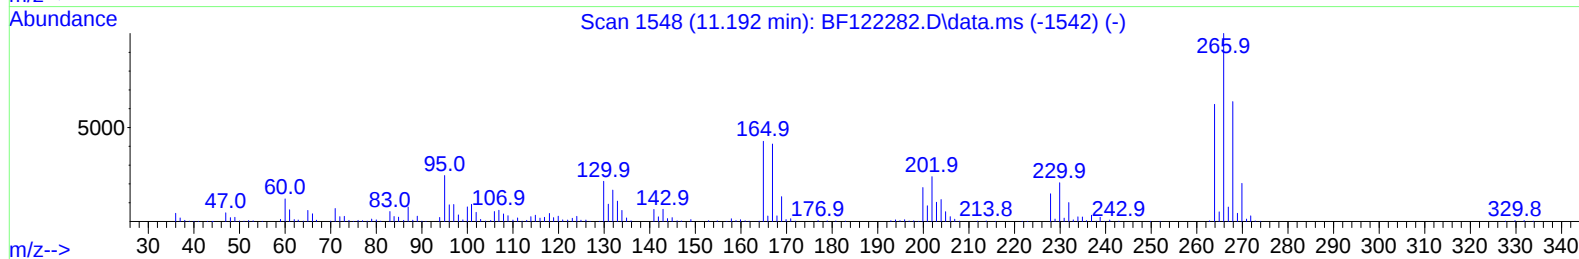
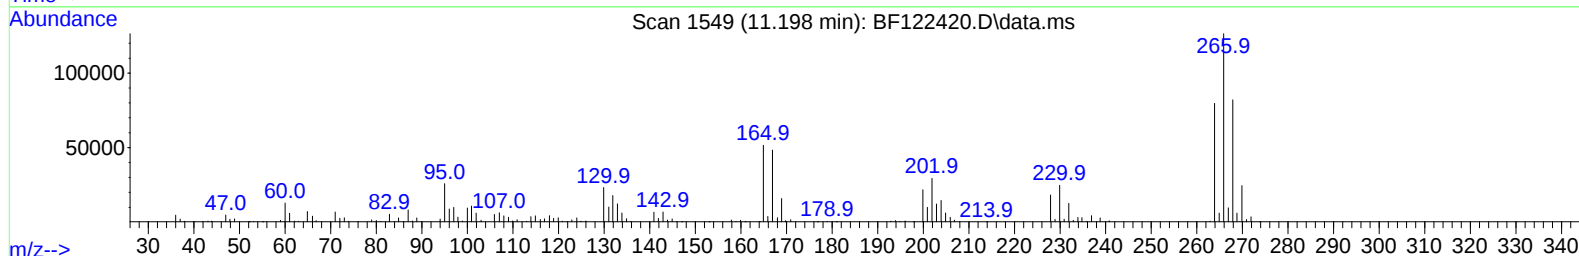


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
Data File : BF122420.D
Acq On : 21 Nov 2020 14:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 03:38:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

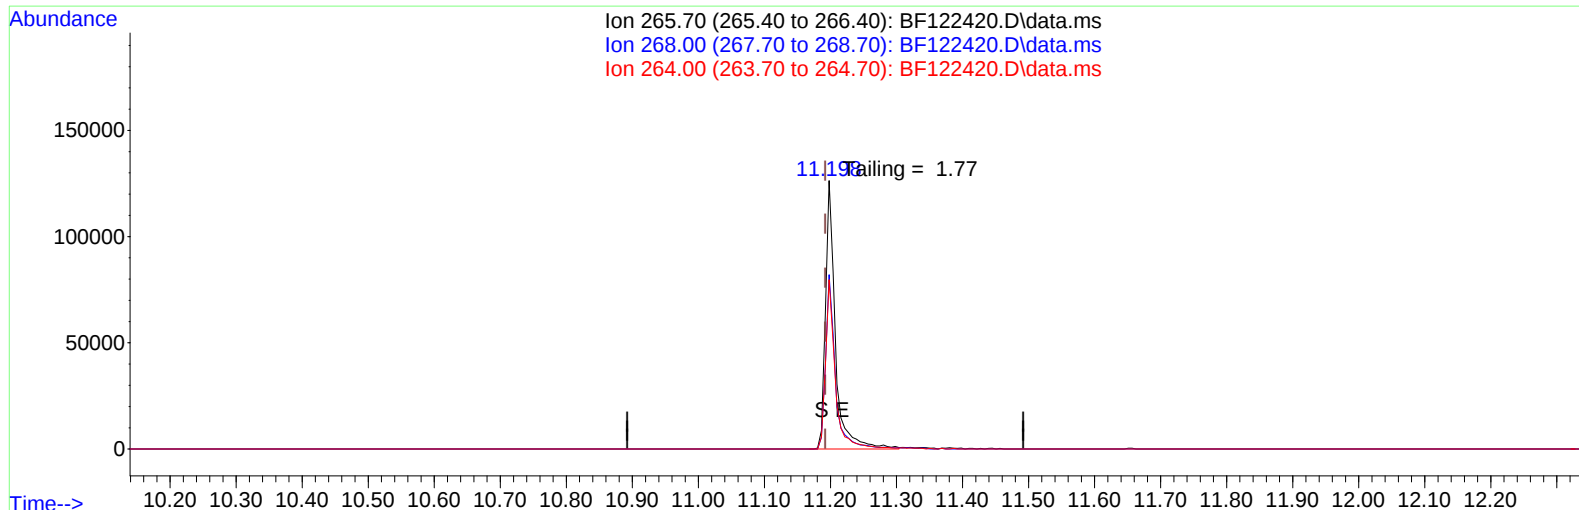

TIC: BF122420.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.006) 37861.13 ng

response 133210

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.93
264.00	62.40	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
Data File : BF122420.D
Acq On : 21 Nov 2020 14:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 03:38:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

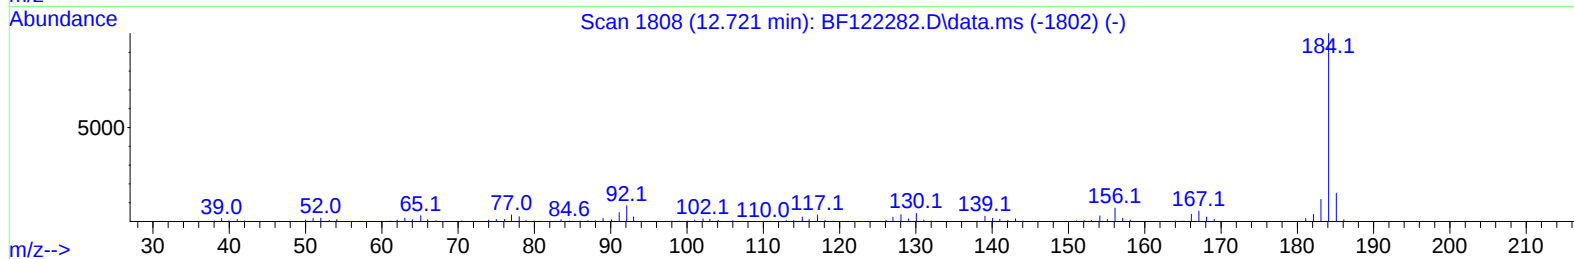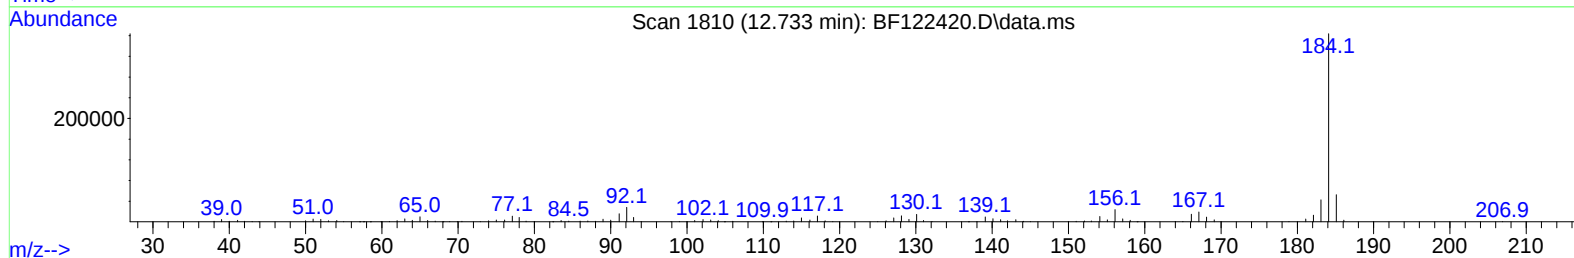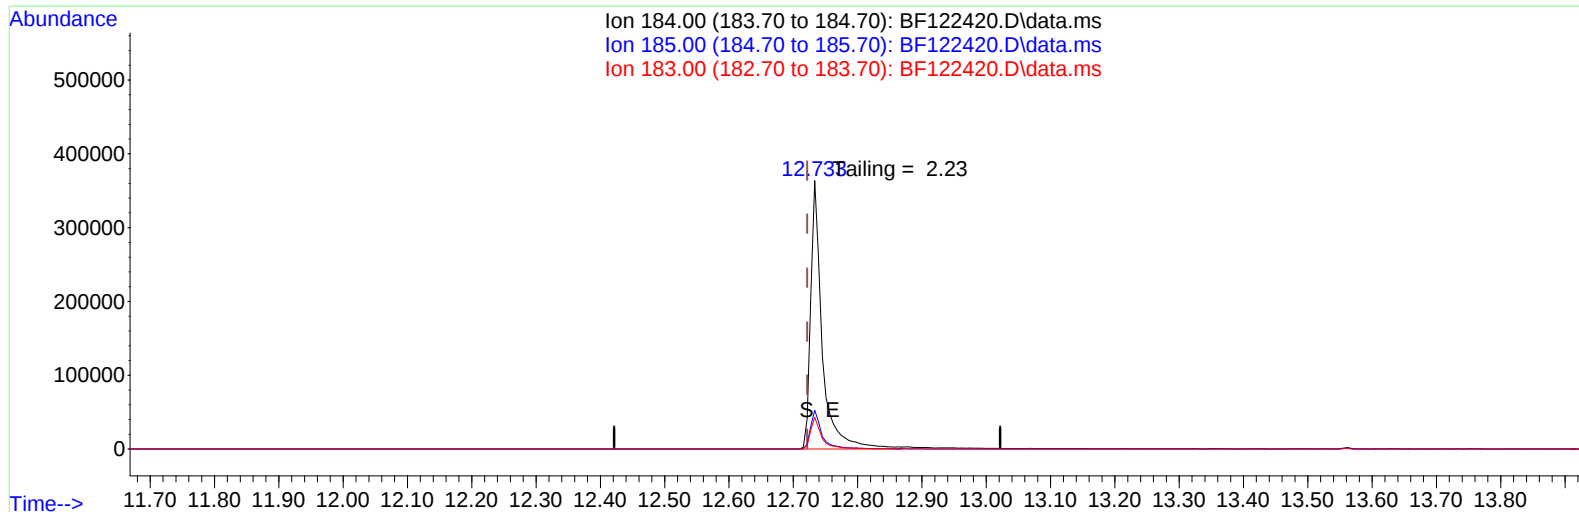

TIC: BF122420.D\data.ms

(77) Benzidine

12.733min (+ 0.012) 0.00 ng

response 463951

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.43
183.00	11.70	11.76
0.00	0.00	0.00