

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
 Data File : BF122424.D
 Acq On : 21 Nov 2020 17:04
 Operator : JU/CG
 Sample : L4800-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FIELD-BLANK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	5	11	44	rVB	2066588	3911397	42.43%	6.266%
2	5.481	573	577	590	rBV	2810152	2606735	28.28%	4.176%
3	6.487	744	748	756	rBV	1801116	1693041	18.37%	2.712%
4	6.863	808	812	815	rBV	1476397	1189360	12.90%	1.905%
5	7.428	902	908	911	rBV	3913283	3920604	42.53%	6.281%
6	8.151	1026	1031	1034	rBV	1563066	1476411	16.02%	2.365%
7	9.228	1209	1214	1217	rBV	6942012	6723417	72.94%	10.772%
8	9.622	1276	1281	1284	rBV	269565	248358	2.69%	0.398%
9	9.904	1325	1329	1333	rBV	1892015	1737421	18.85%	2.784%
10	10.698	1459	1464	1467	rBV	3914610	3618510	39.26%	5.797%
11	11.392	1578	1582	1586	rBV	2119658	1910591	20.73%	3.061%
12	11.939	1664	1675	1694	rBV	3701453	6757347	73.31%	10.826%
13	12.192	1715	1718	1725	rVB	166470	180791	1.96%	0.290%
14	12.580	1781	1784	1787	rBV	213490	258781	2.81%	0.415%
15	12.645	1787	1795	1798	rVV5	184237	514174	5.58%	0.824%
16	12.727	1802	1809	1820	rVV	5114294	9217644	100.00%	14.768%
17	12.804	1820	1822	1830	rVB2	184634	292848	3.18%	0.469%
18	12.992	1848	1854	1857	rBV	7611718	7819404	84.83%	12.528%
19	13.222	1889	1893	1897	rBV	88103	97816	1.06%	0.157%
20	13.516	1939	1943	1946	rBV	177297	198436	2.15%	0.318%
21	13.892	2003	2007	2021	rBV	794231	1226041	13.30%	1.964%
22	14.039	2028	2032	2040	rVB	2176639	1903239	20.65%	3.049%
23	14.210	2058	2061	2064	rBV	135176	119018	1.29%	0.191%
24	14.516	2108	2113	2115	rBV2	168829	172864	1.88%	0.277%
25	14.716	2135	2147	2158	rBV4	298927	1250105	13.56%	2.003%
26	14.827	2163	2166	2175	rVV	174258	261112	2.83%	0.418%
27	14.904	2175	2179	2184	rVB	991882	1029514	11.17%	1.649%
28	15.168	2221	2224	2228	rBV	103471	121965	1.32%	0.195%
29	15.515	2278	2283	2288	rBV	1347299	1707012	18.52%	2.735%
30	15.557	2288	2290	2298	rVB	73024	101001	1.10%	0.162%
31	16.074	2374	2378	2386	rBV5	54342	152760	1.66%	0.245%




Sum of corrected areas: 62417717

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
Data File : BF122424.D
Acq On : 21 Nov 2020 17:04
Operator : JU/CG
Sample : L4800-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

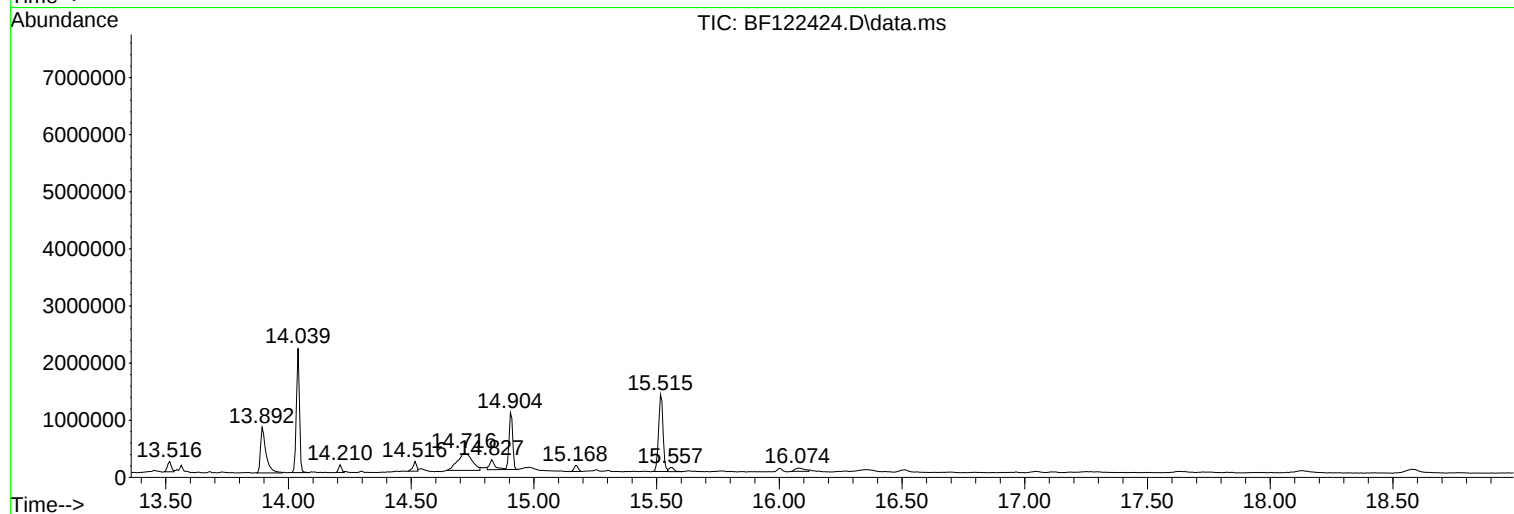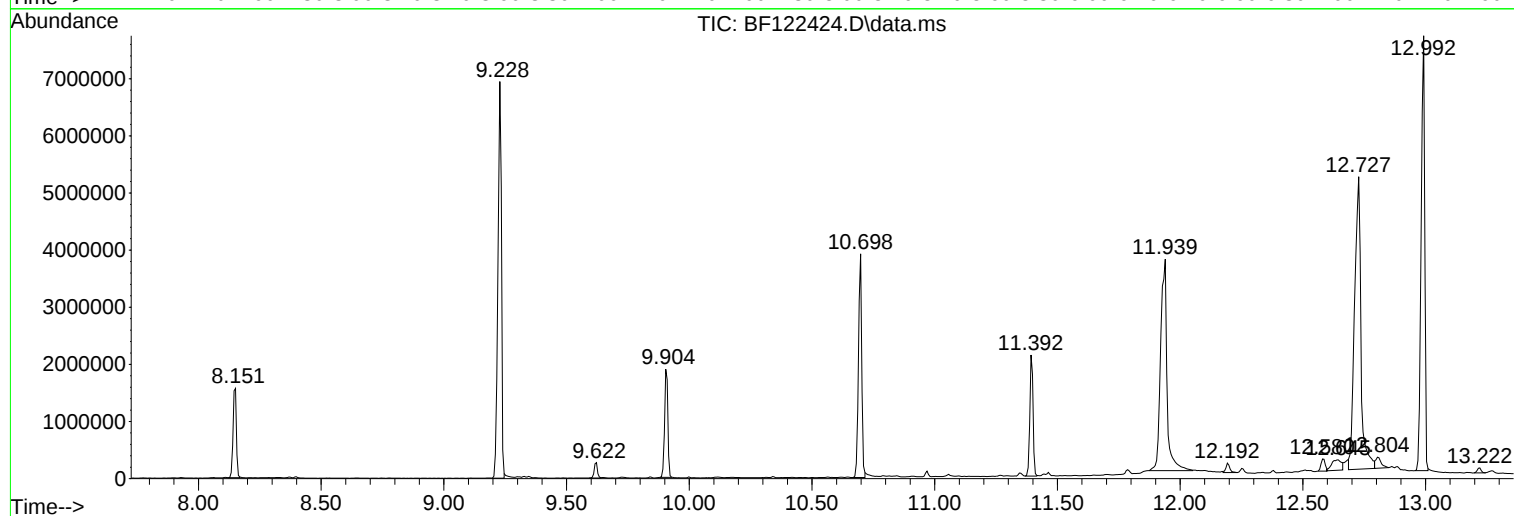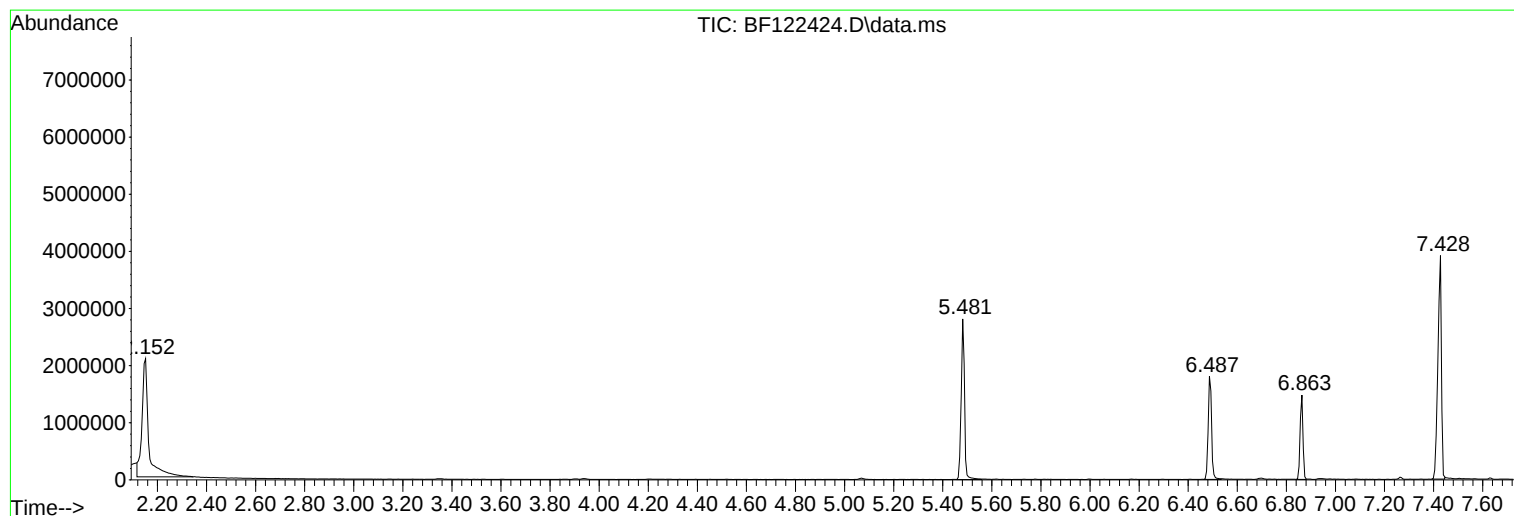

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
Data File : BF122424.D
Acq On : 21 Nov 2020 17:04
Operator : JU/CG
Sample : L4800-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
Data File : BF122424.D
Acq On : 21 Nov 2020 17:04
Operator : JU/CG
Sample : L4800-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
