
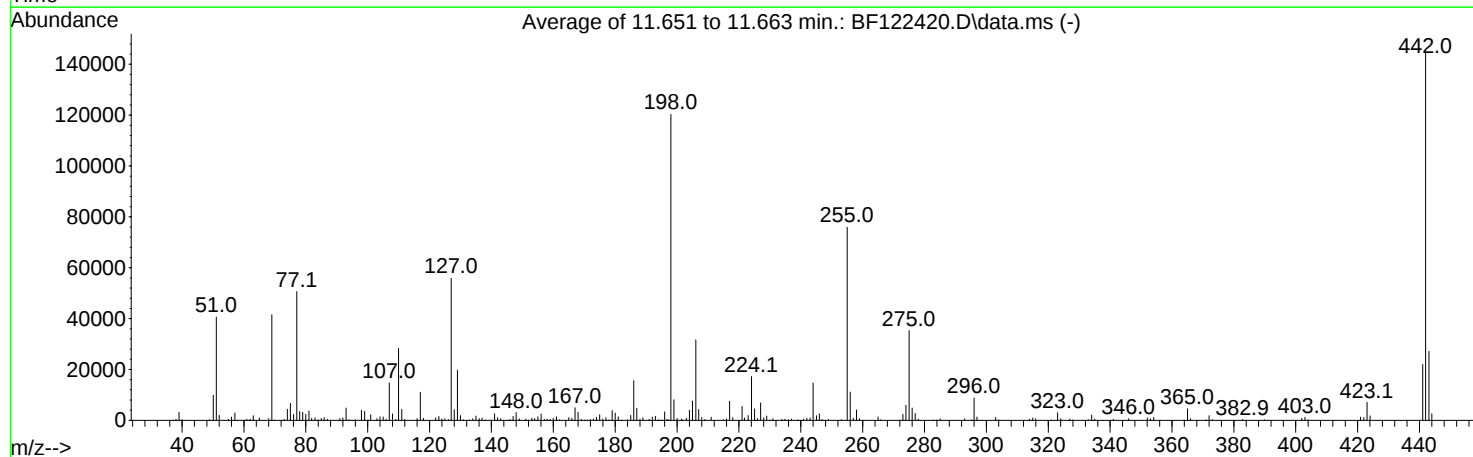


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112120\
 Data File : BF122420.D
 Acq On : 21 Nov 2020 14:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 13:27:02 2020

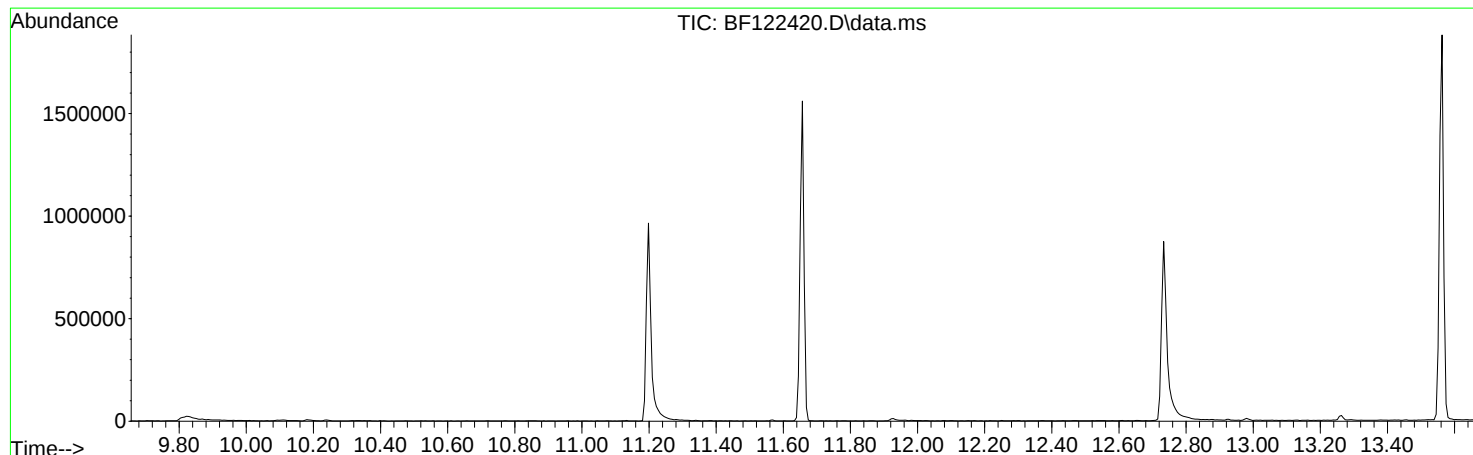

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	40581	PASS
68	69	0.00	2	1.7	700	PASS
69	198	0.00	100	34.5	41518	PASS
70	69	0.00	2	0.3	107	PASS
127	198	10	80	46.5	55869	PASS
197	198	0.00	2	0.3	395	PASS
198	198	100	100	100.0	120275	PASS
199	198	5	9	6.8	8121	PASS
275	198	10	60	29.3	35269	PASS
365	198	1	100	3.8	4538	PASS
441	198	0.01	100	18.3	21986	PASS
442	442	100	100	100.0	144621	PASS
443	442	15	24	18.8	27136	PASS