
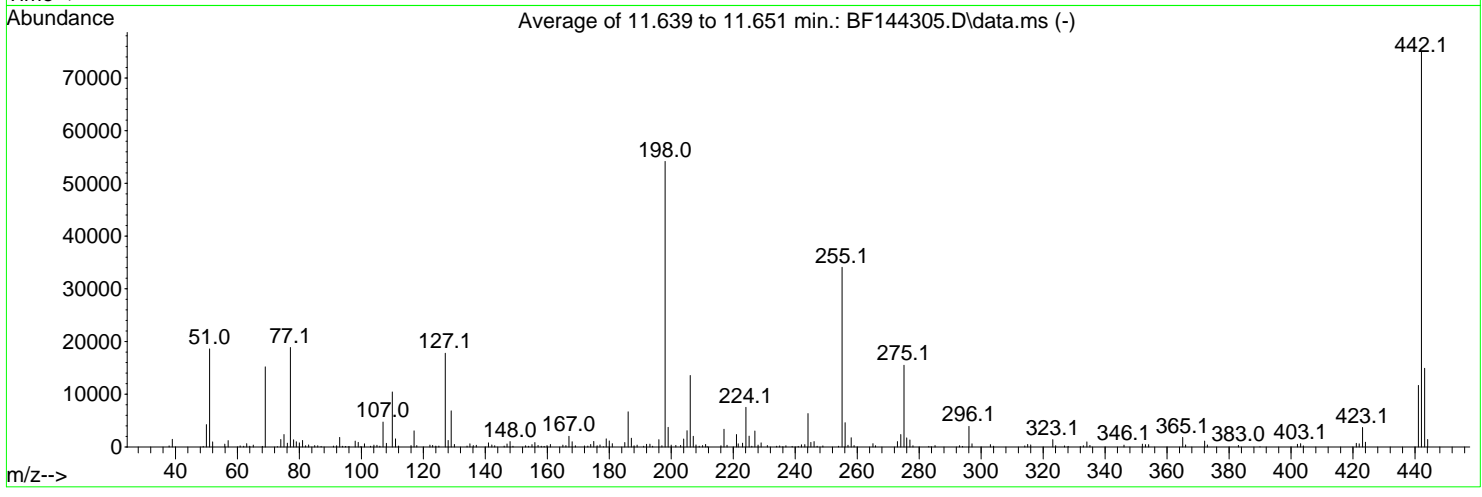


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112125\
 Data File : BF144305.D
 Acq On : 21 Nov 2025 12:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 05 18:37:33 2025

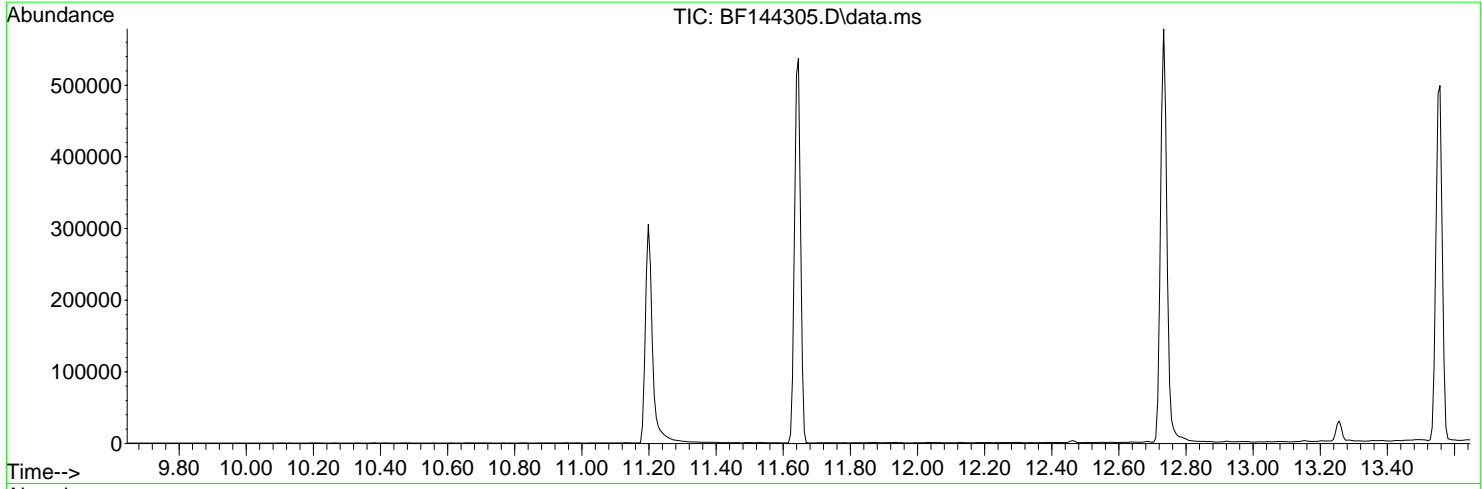




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.8	118	PASS
69	69	100	100	100.0	15198	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	243	PASS
198	198	100	100	100.0	54171	PASS
199	198	5	9	6.9	3729	PASS
365	198	1	100	3.3	1803	PASS
441	443	0.01	150	78.3	11677	PASS
442	442	100	100	100.0	74909	PASS
443	442	15	24	19.9	14915	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112125\
 Data File : BF144305.D
 Acq On : 21 Nov 2025 12:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Quant Time: Nov 21 13:19:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 05 18:37:33 2025
 Response via : Initial Calibration

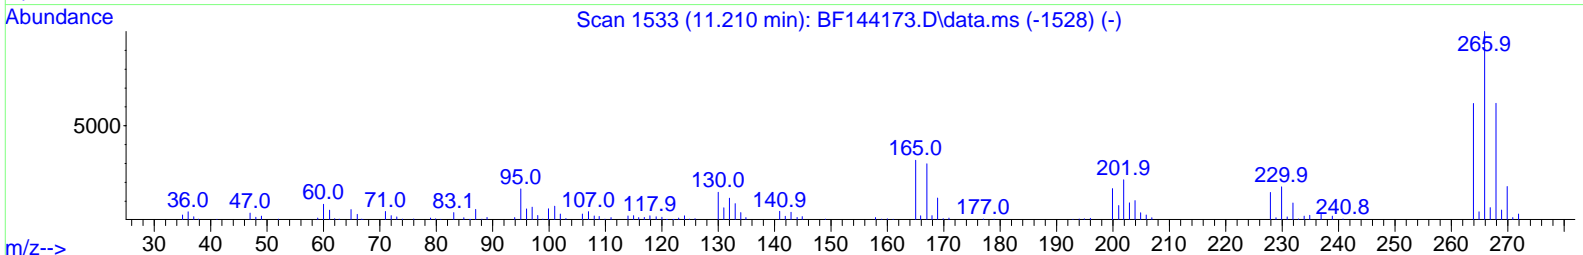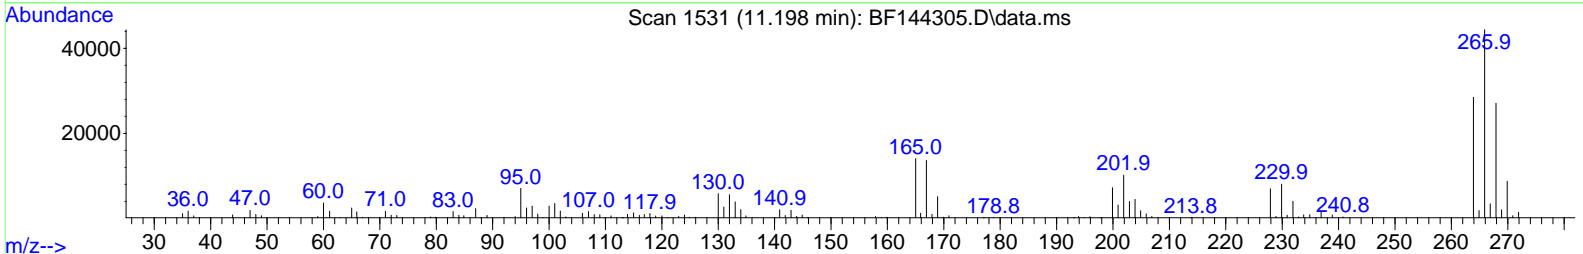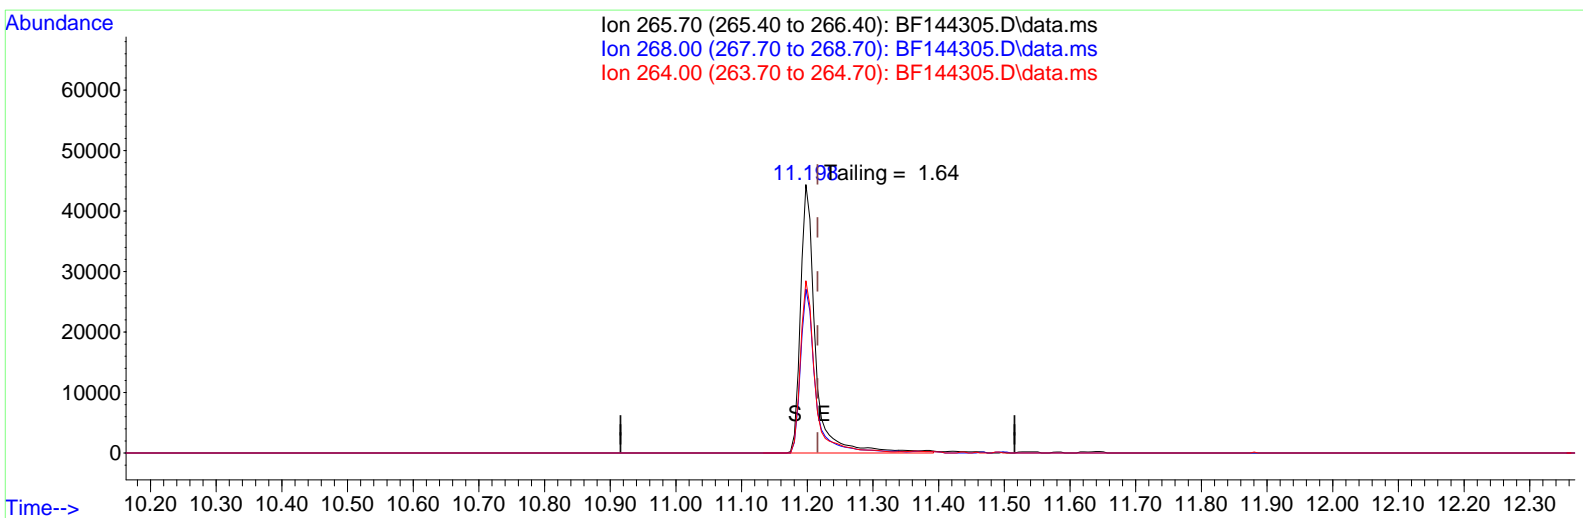

TIC: BF144305.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.018) 29964.57 ng

response	69767	
Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.03
264.00	61.80	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112125\
 Data File : BF144305.D
 Acq On : 21 Nov 2025 12:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 21 13:19:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 05 18:37:33 2025
 Response via : Initial Calibration

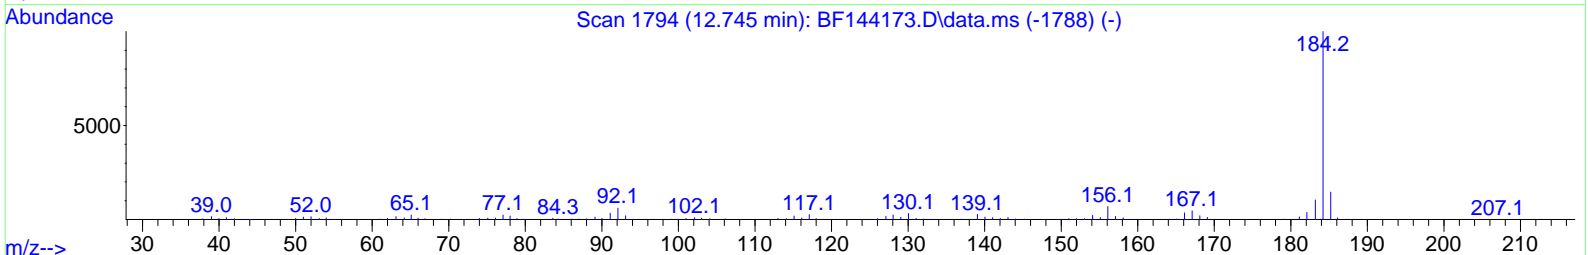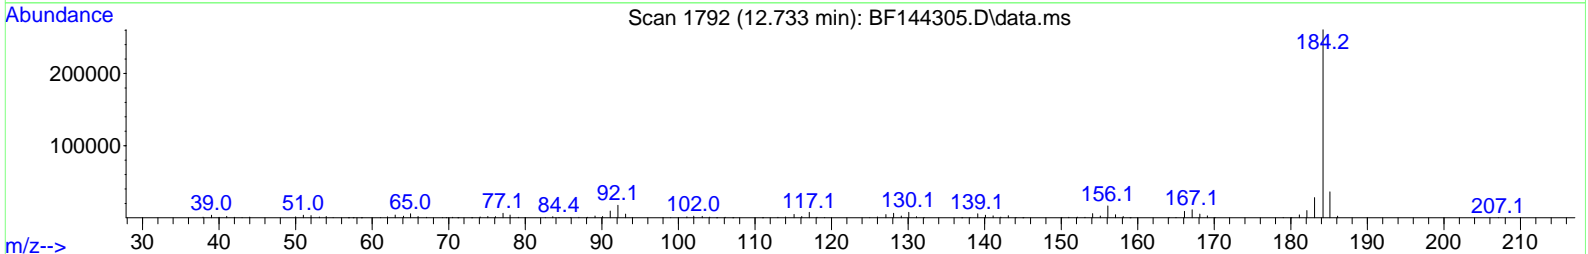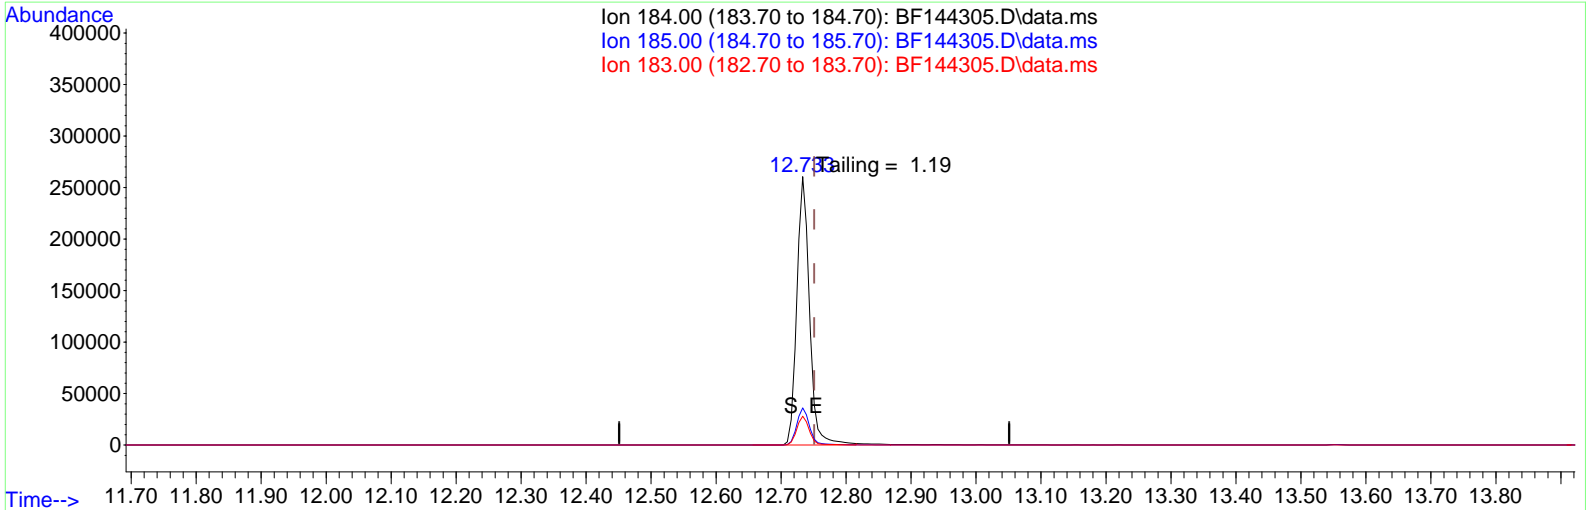

TIC: BF144305.D\data.ms

(77) Benzidine

12.733min (-0.018) 0.00 ng

response 357229

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.87
183.00	10.40	10.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2025	BNA_F	<u>BF144305.D</u>
Compound Name	Response	Retention Time
DDT	142530	13.557
DDD		13.257
DDE	411	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
411	142941	0.29

Instrument :
 BNA_F
 ClientSampled :
 DFTPP