
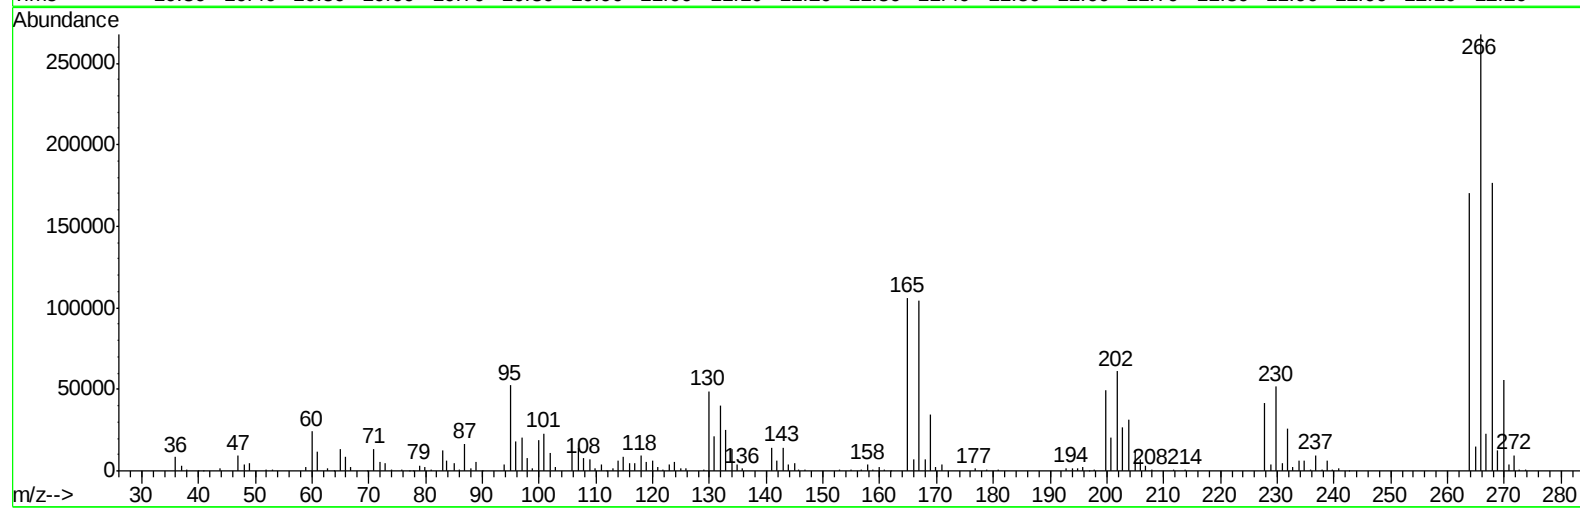


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112219\
Data File : BF117924.D
Acq On : 22 Nov 2019 18:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 03:45:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

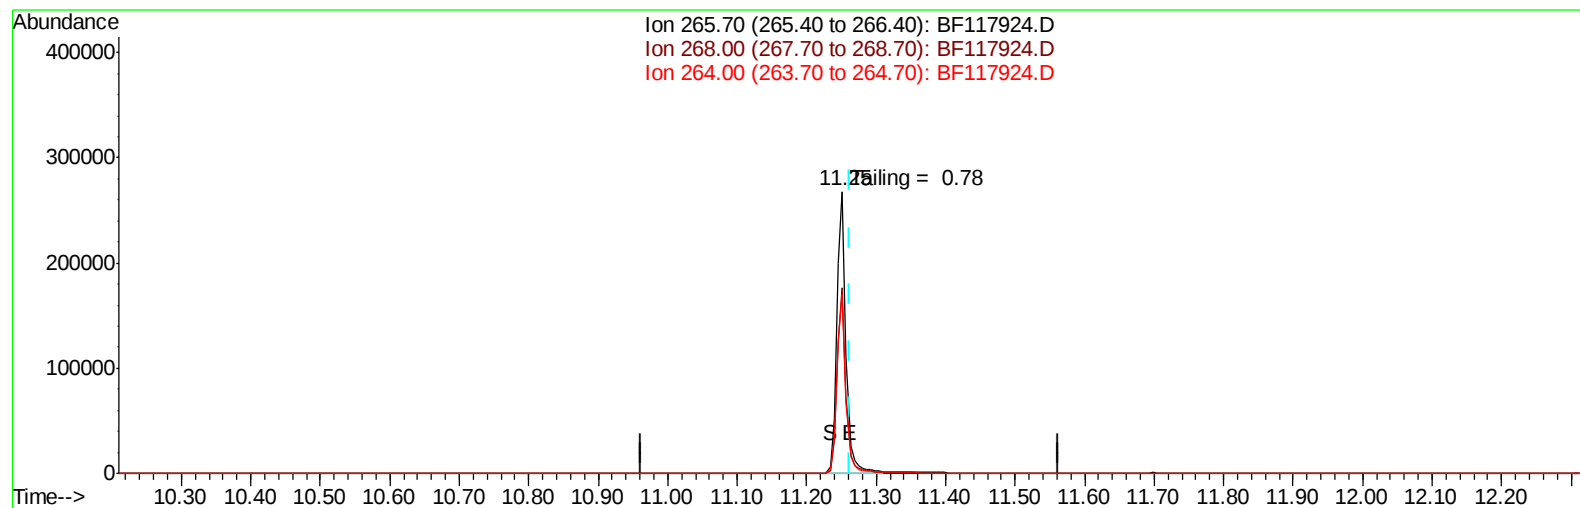

TIC: BF117924.D

(70) Pentachlorophenol (C)



11.251min (-0.012) 72826.88ng

response 247851

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.85
264.00	63.40	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112219\
Data File : BF117924.D
Acq On : 22 Nov 2019 18:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 03:45:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

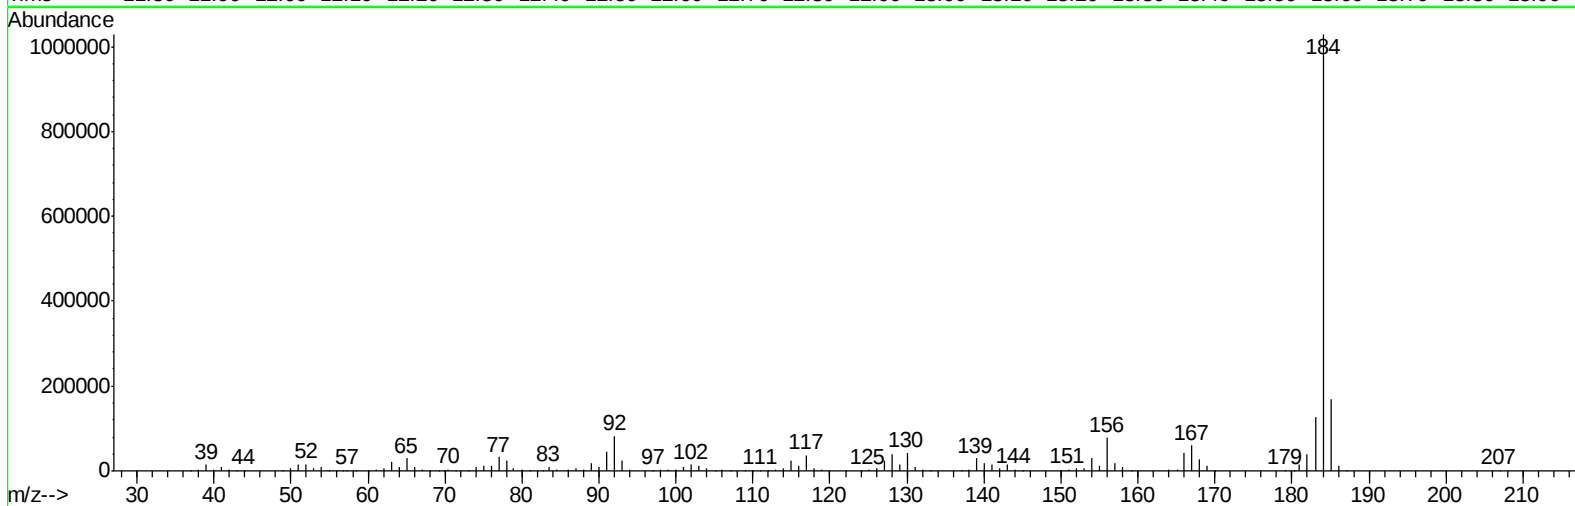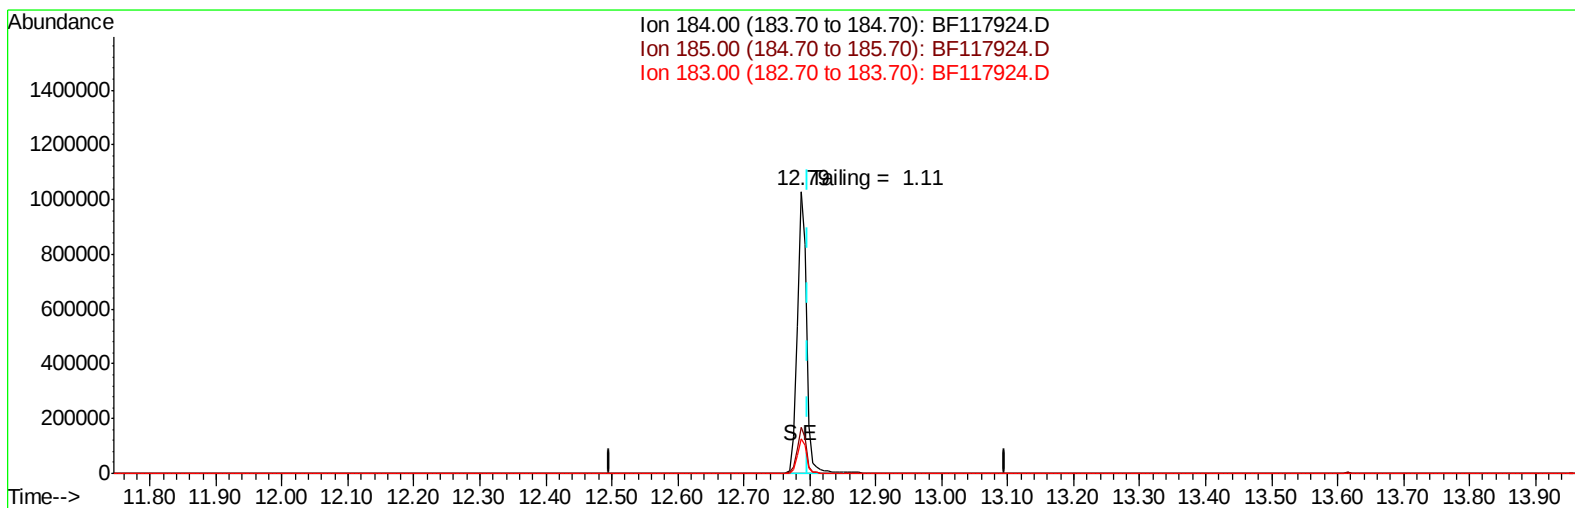

TIC: BF117924.D

(77) Benzidine

12.786min (-0.011) 273873.18ng

response 1013717

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	16.37
183.00	11.90	12.26
0.00	0.00	0.00