


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112219\
 Data File : BF117924.D
 Acq On : 22 Nov 2019 18:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

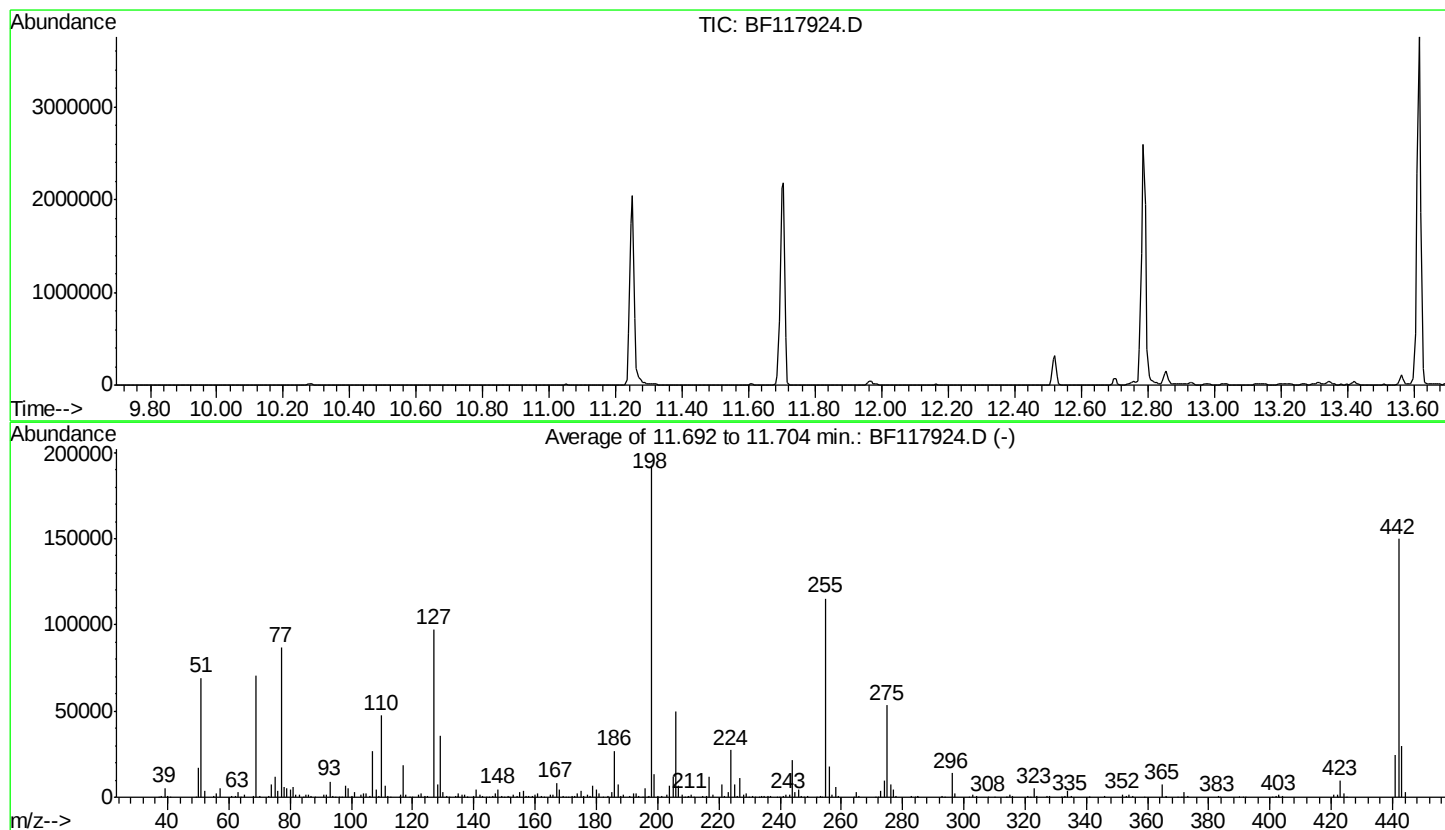

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	69181	PASS
68	69	0.00	2	1.5	1067	PASS
69	198	0.00	100	36.5	70234	PASS
70	69	0.00	2	0.7	480	PASS
127	198	10	80	50.6	97261	PASS
197	198	0.00	2	0.3	655	PASS
198	198	100	100	100.0	192349	PASS
199	198	5	9	6.8	13078	PASS
275	198	10	60	27.7	53277	PASS
365	198	1	100	3.7	7187	PASS
441	198	0.01	100	12.8	24612	PASS
442	198	50	100	77.9	149770	PASS
443	442	15	24	20.0	29958	PASS