


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112319\
 Data File : BF117949.D
 Acq On : 23 Nov 2019 11:55
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

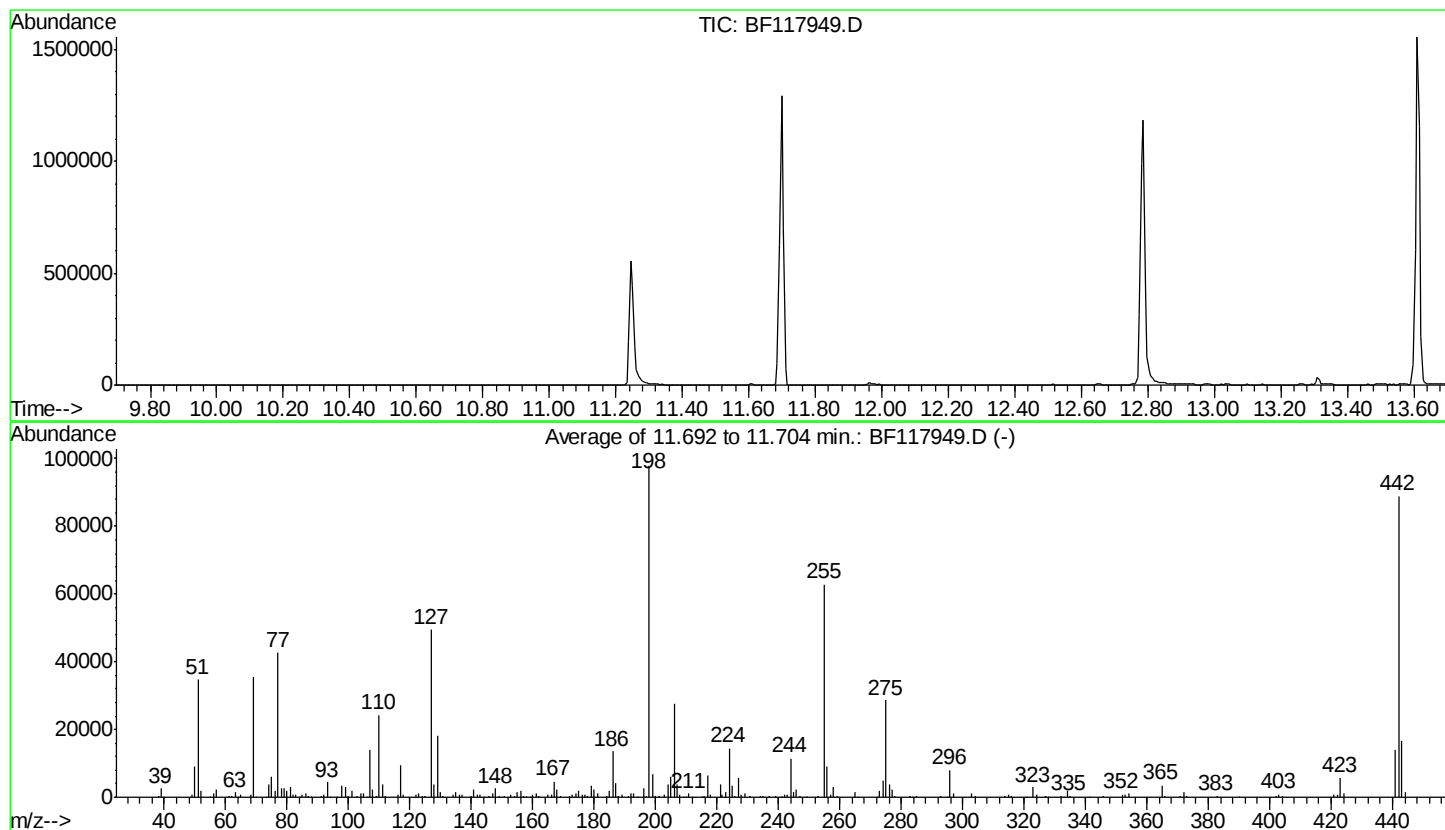

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	34645	PASS
68	69	0.00	2	1.9	663	PASS
69	198	0.00	100	36.2	35482	PASS
70	69	0.00	2	0.3	103	PASS
127	198	10	80	50.4	49349	PASS
197	198	0.00	2	0.2	205	PASS
198	198	100	100	100.0	97901	PASS
199	198	5	9	7.0	6892	PASS
275	198	10	60	29.3	28650	PASS
365	198	1	100	3.7	3578	PASS
441	198	0.01	100	14.3	14008	PASS
442	198	50	100	90.8	88901	PASS
443	442	15	24	18.7	16658	PASS