
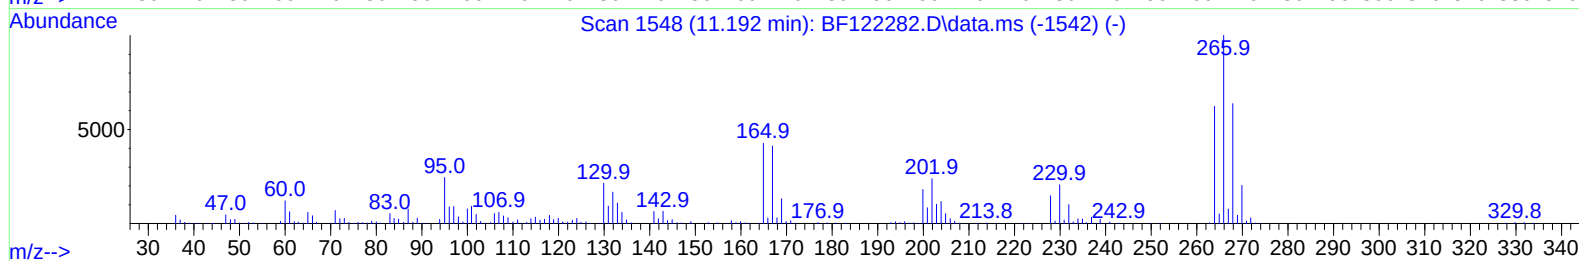
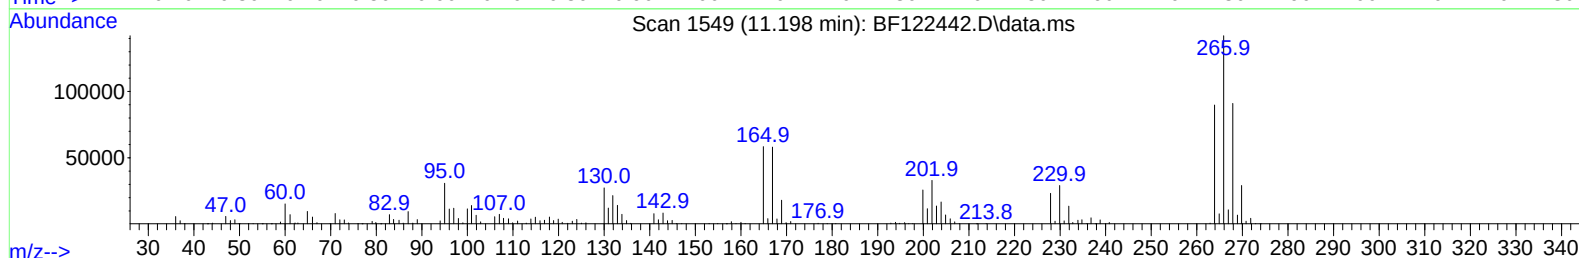


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112320\  
Data File : BF122442.D  
Acq On    : 23 Nov 2020  12:05  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 25 06:33:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

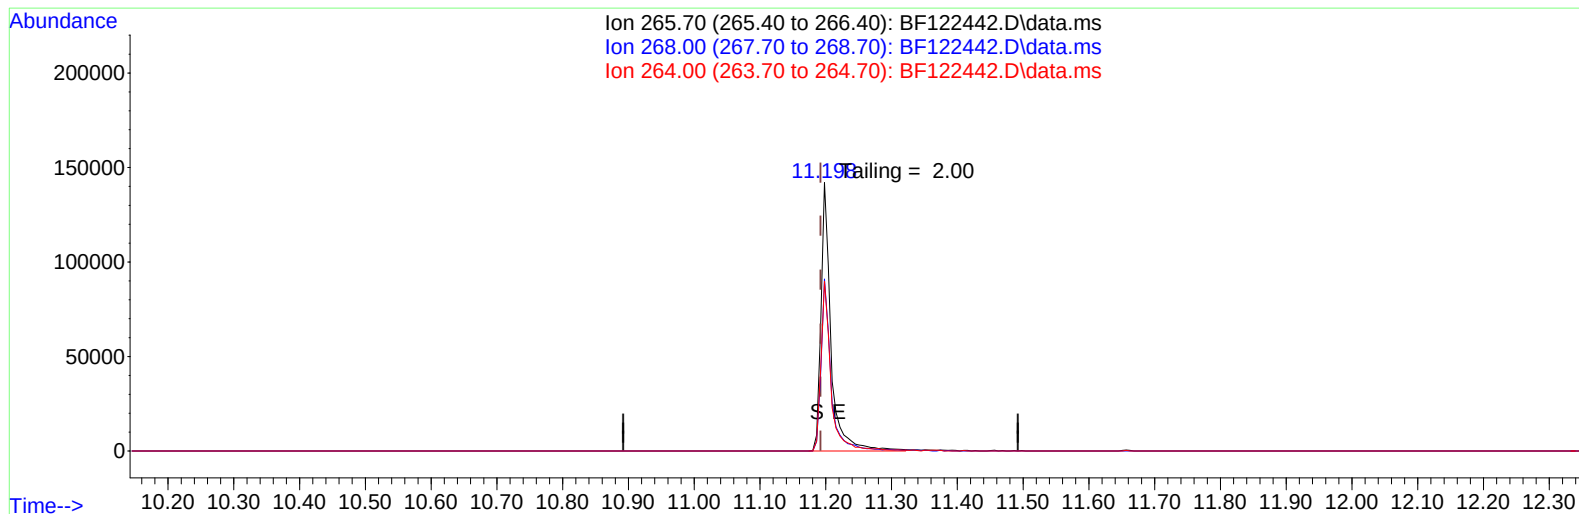

TIC: BF122442.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.006) 32429.91 ng

response **151581**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.09
264.00	62.40	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112320\
Data File : BF122442.D
Acq On : 23 Nov 2020 12:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 06:33:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

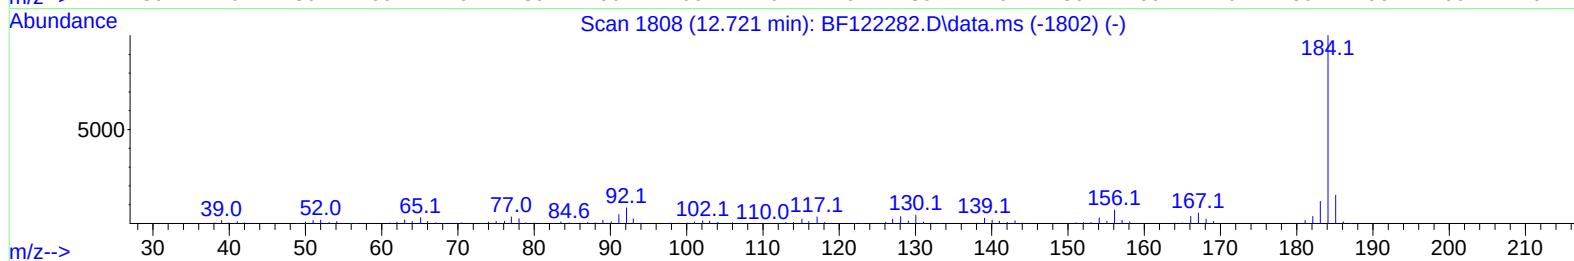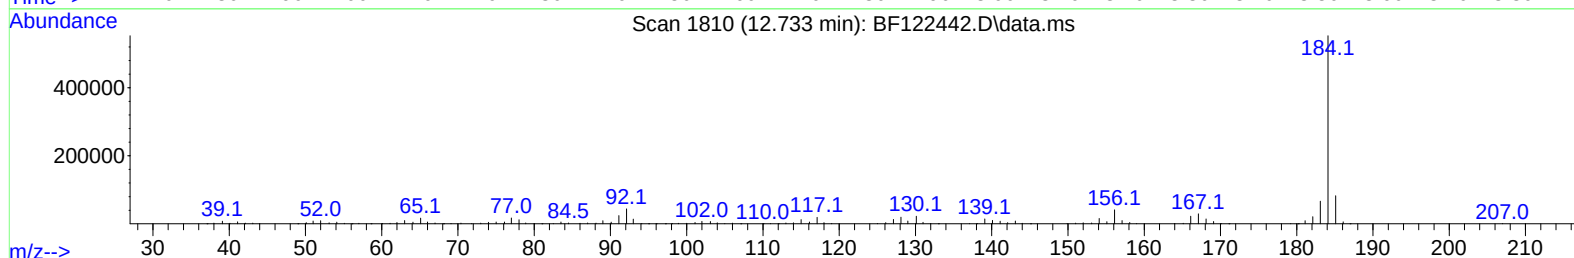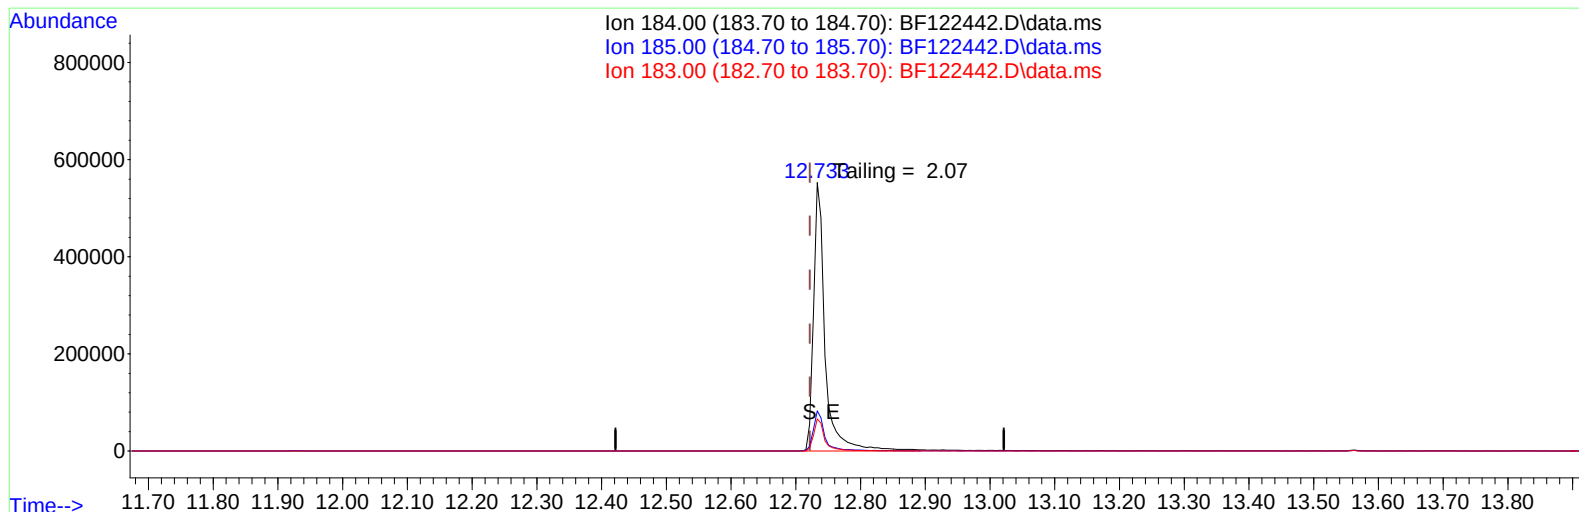

TIC: BF122442.D\data.ms

(77) Benzidine

12.733min (+ 0.012) 0.00 ng

response 688264

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.98
183.00	11.70	12.02
0.00	0.00	0.00