


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112320\
Data File : BF122442.D
Acq On : 23 Nov 2020 12:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 20 13:27:02 2020

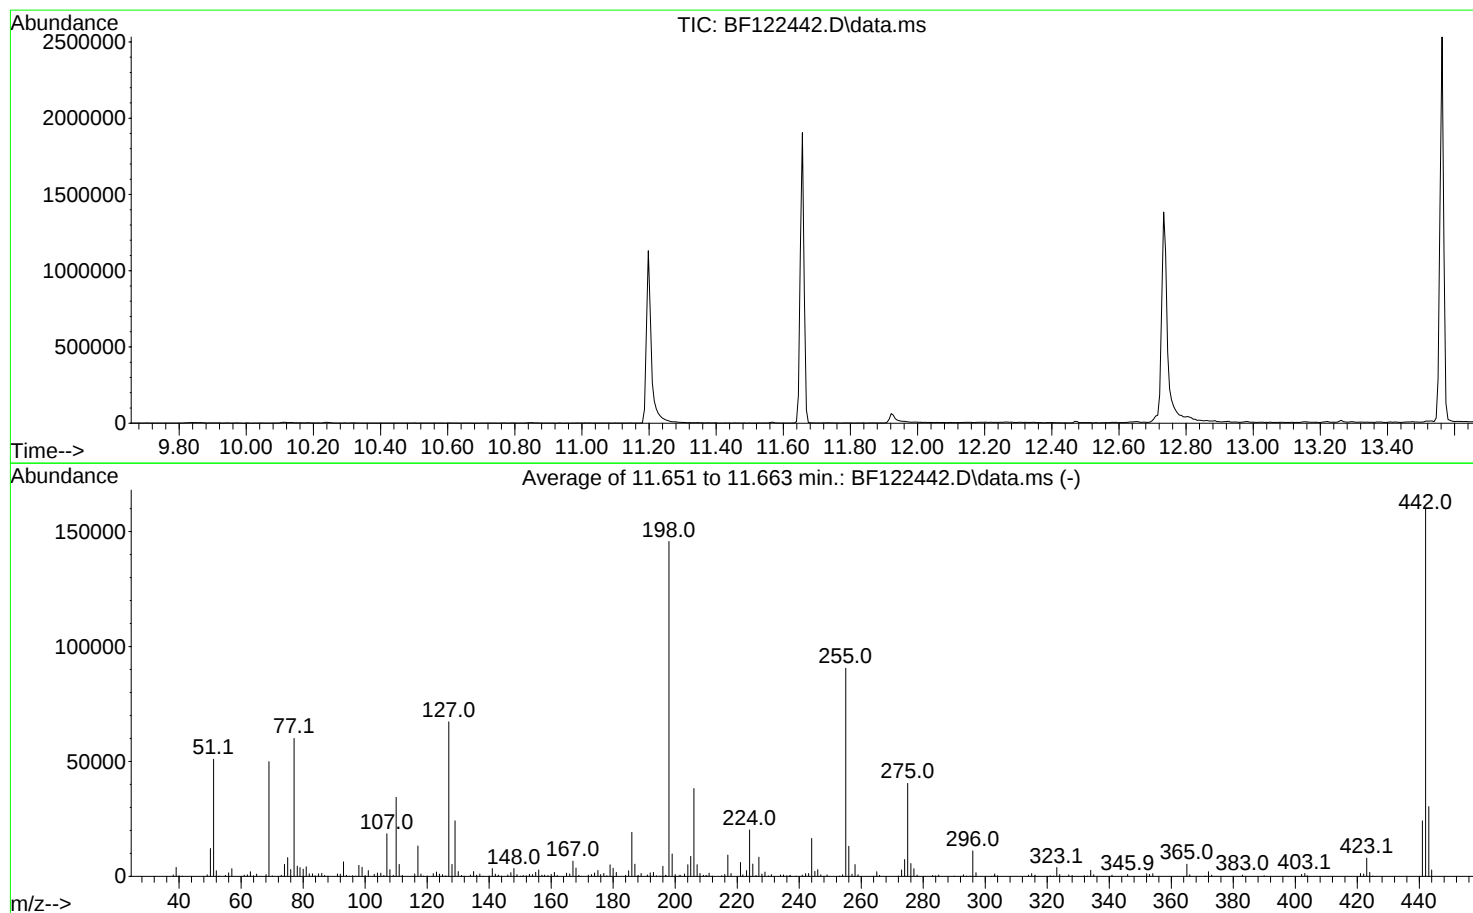

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	50989	PASS
68	69	0.00	2	1.6	795	PASS
69	198	0.00	100	34.3	49920	PASS
70	69	0.00	2	0.5	237	PASS
127	198	10	80	46.1	67227	PASS
197	198	0.00	2	0.4	516	PASS
198	198	100	100	100.0	145725	PASS
199	198	5	9	6.7	9728	PASS
275	198	10	60	27.8	40459	PASS
365	198	1	100	3.7	5323	PASS
441	198	0.01	100	16.6	24187	PASS
442	442	100	100	100.0	160051	PASS
443	442	15	24	19.0	30362	PASS