
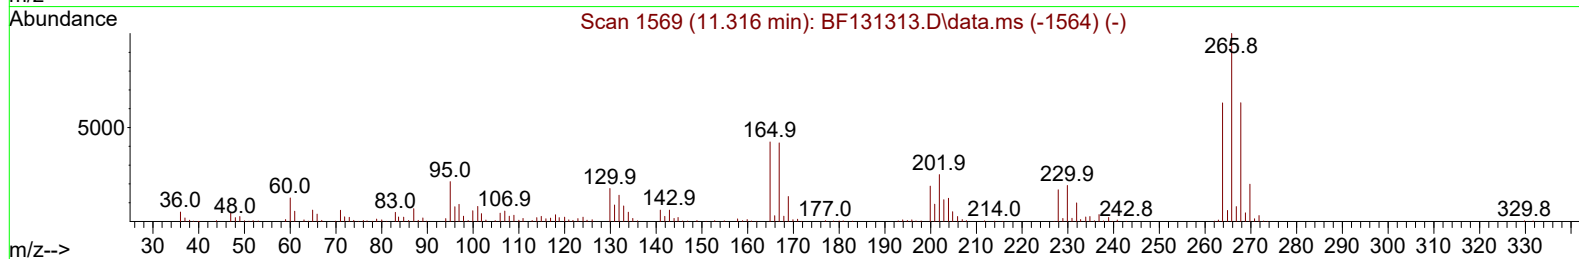
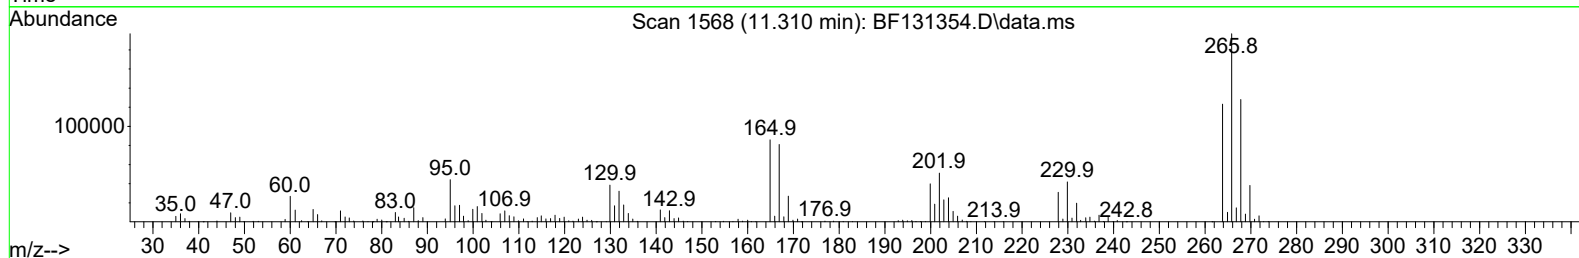


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112322\
Data File : BF131354.D
Acq On : 23 Nov 2022 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 07:18:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:53:32 2022
Response via : Initial Calibration

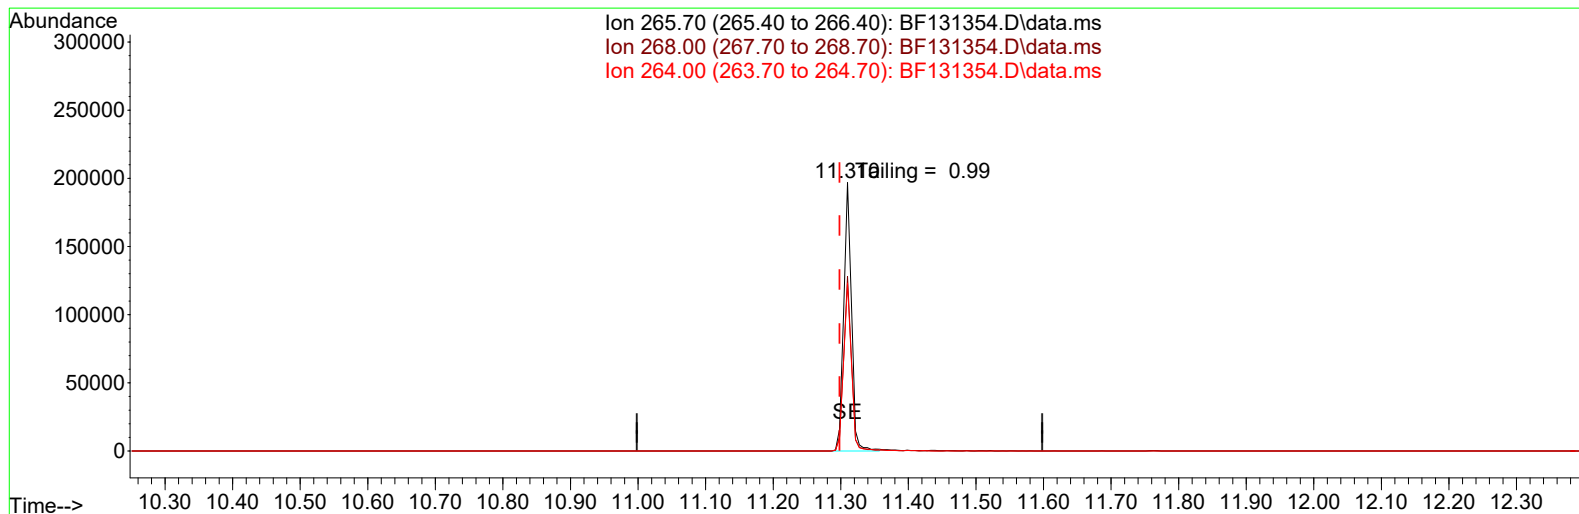

TIC: BF131354.D\data.ms

(70) Pentachlorophenol (C)




11.310min (+ 0.012) 32798.69 ng

response 159438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	65.04
264.00	63.00	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112322\
Data File : BF131354.D
Acq On : 23 Nov 2022 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 07:18:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:53:32 2022
Response via : Initial Calibration

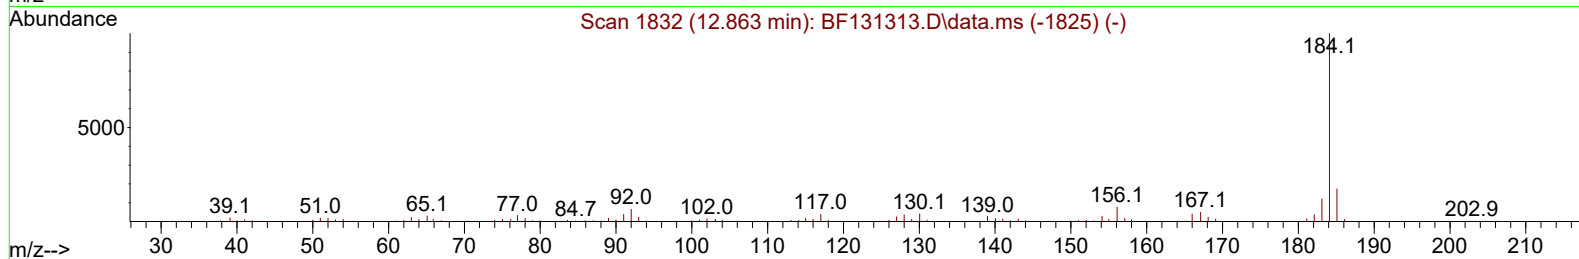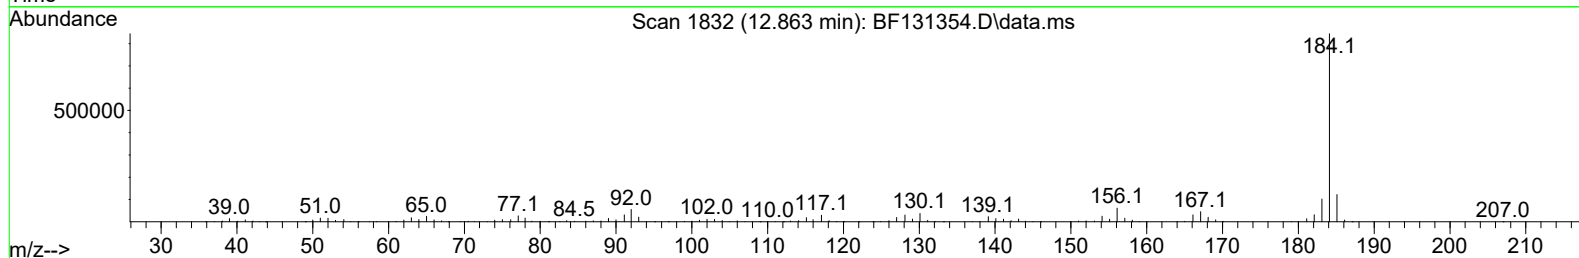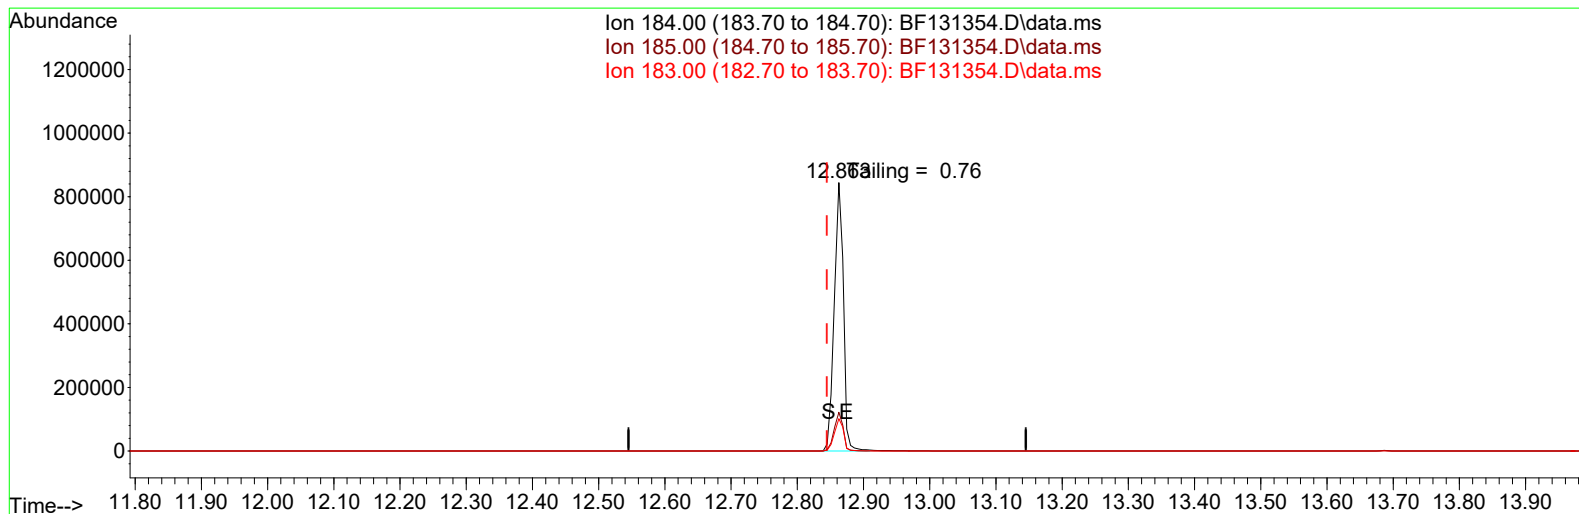

TIC: BF131354.D\data.ms

(77) Benzidine

12.863min (+ 0.018) 0.00 ng

response 812496

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.45
183.00	12.00	12.08
0.00	0.00	0.00