


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112322\
Data File : BF131362.D
Acq On : 23 Nov 2022 15:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 24 05:53:32 2022

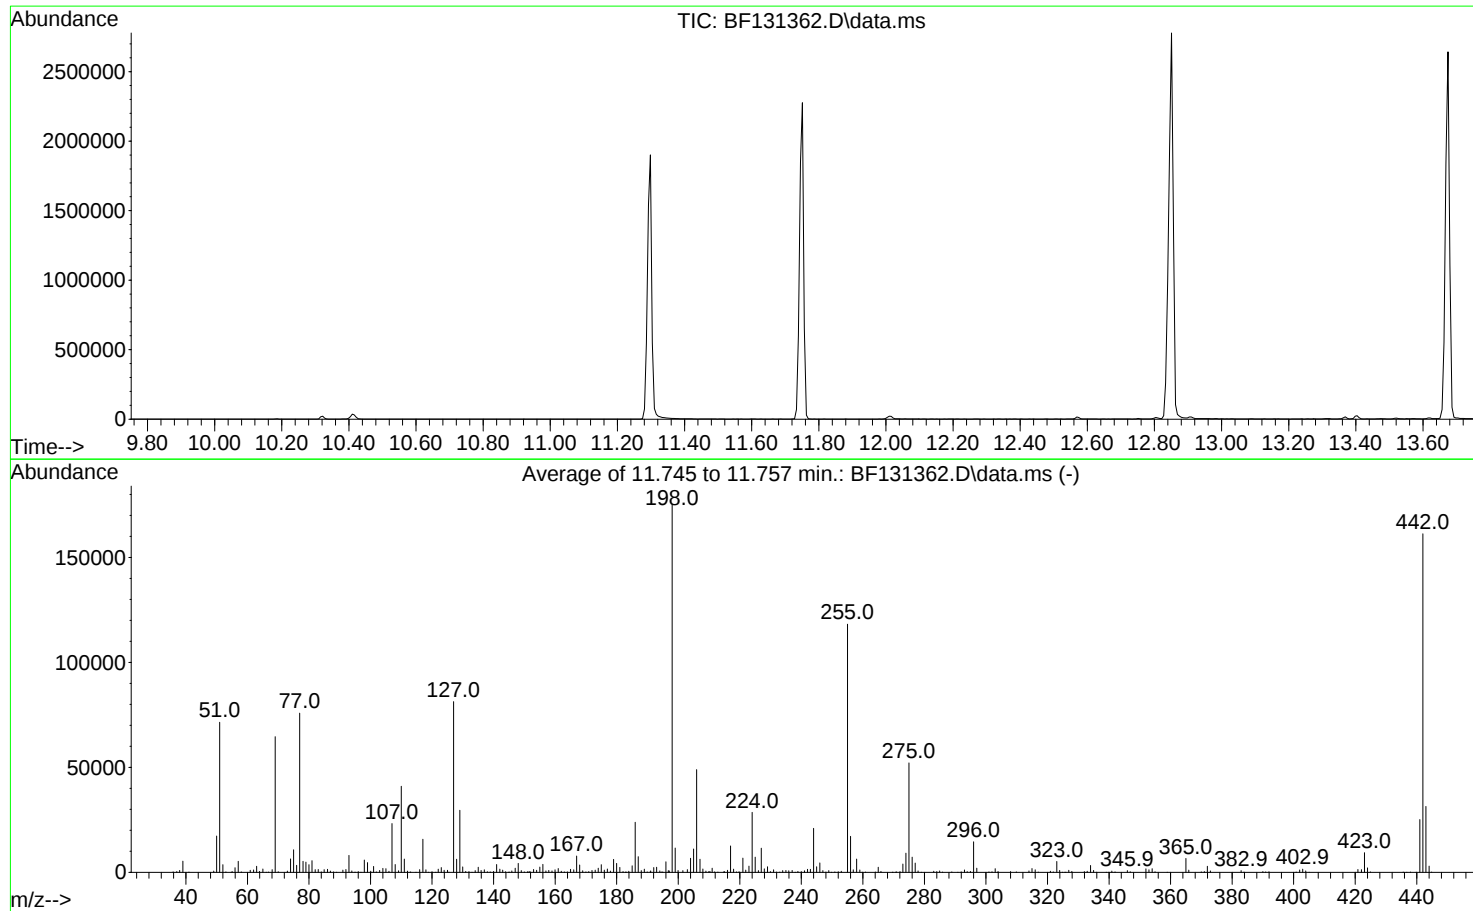




AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	71433	PASS
68	69	0.00	2	1.9	1226	PASS
69	198	0.00	100	36.9	64603	PASS
70	69	0.00	2	0.5	302	PASS
127	198	10	80	46.4	81304	PASS
197	198	0.00	2	0.5	843	PASS
198	198	100	100	100.0	175248	PASS
199	198	5	9	6.6	11569	PASS
275	198	10	60	29.7	52107	PASS
365	198	1	100	3.8	6590	PASS
441	198	0.01	100	14.3	25147	PASS
442	442	50	100	100.0	161280	PASS
443	442	15	24	19.4	31336	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112322\
 Data File : BF131362.D
 Acq On : 23 Nov 2022 15:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 07:23:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 05:53:32 2022
 Response via : Initial Calibration

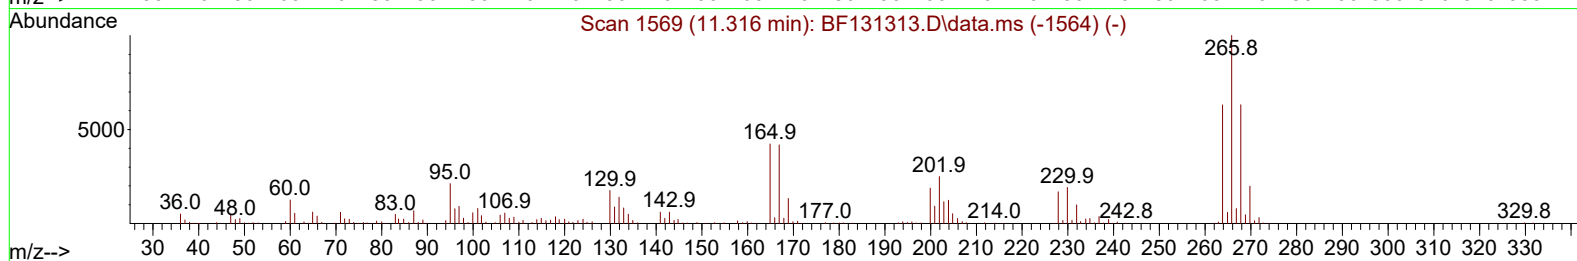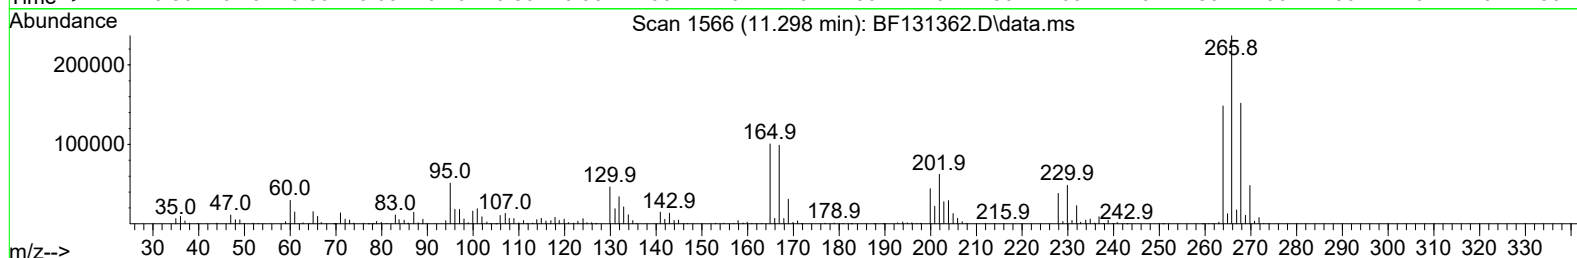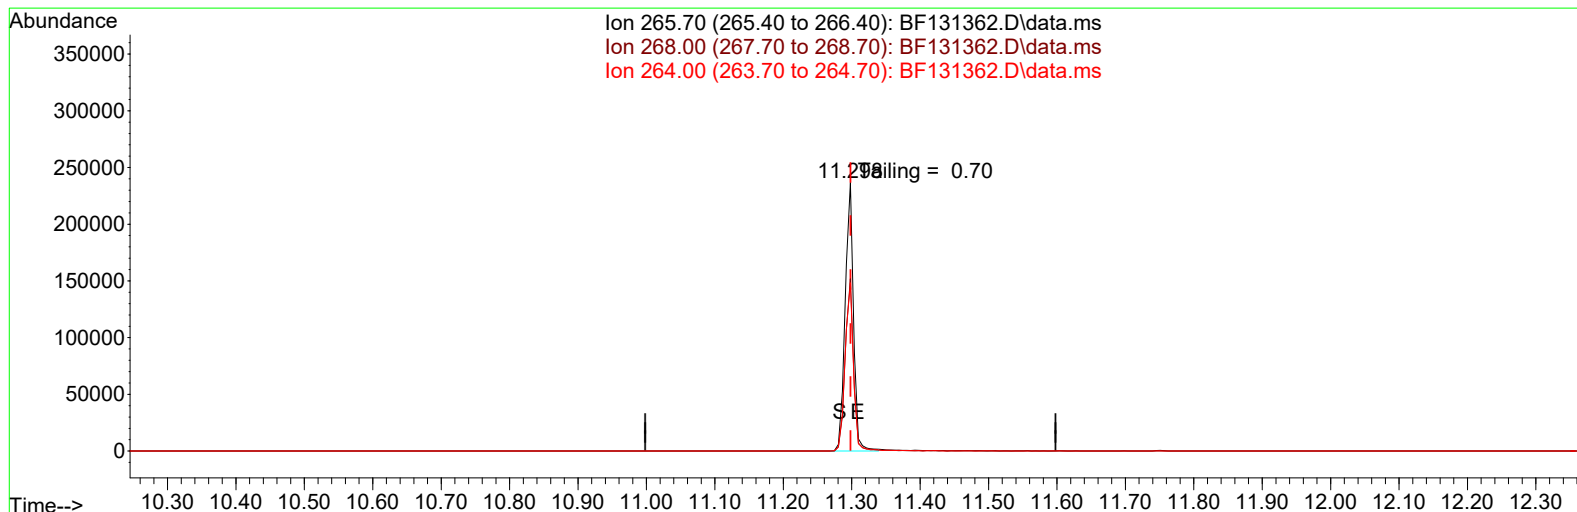

TIC: BF131362.D\data.ms

(70) Pentachlorophenol (C)

11.298min (-0.000) 331110.31 ng




response 202555

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.14
264.00	63.00	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112322\
Data File : BF131362.D
Acq On : 23 Nov 2022 15:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 24 07:23:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:53:32 2022
Response via : Initial Calibration

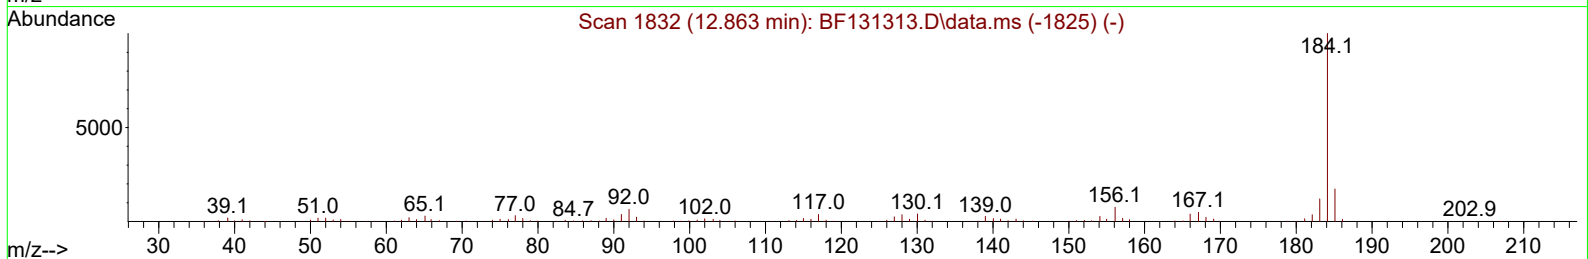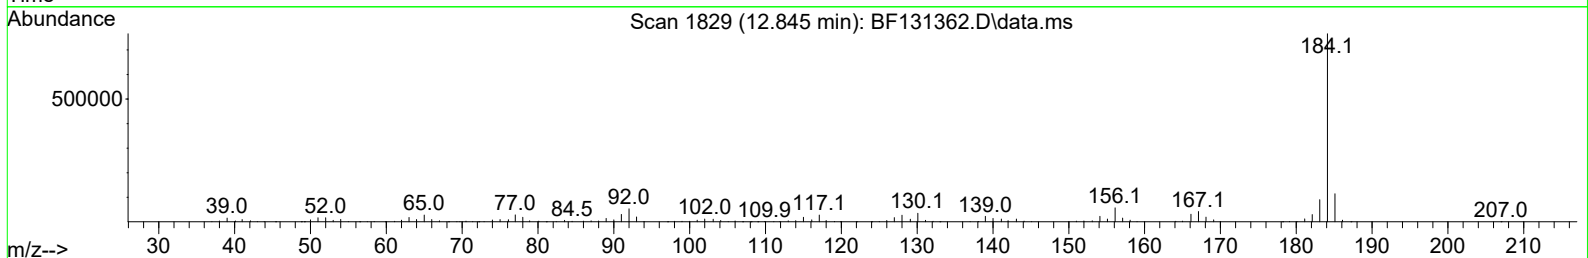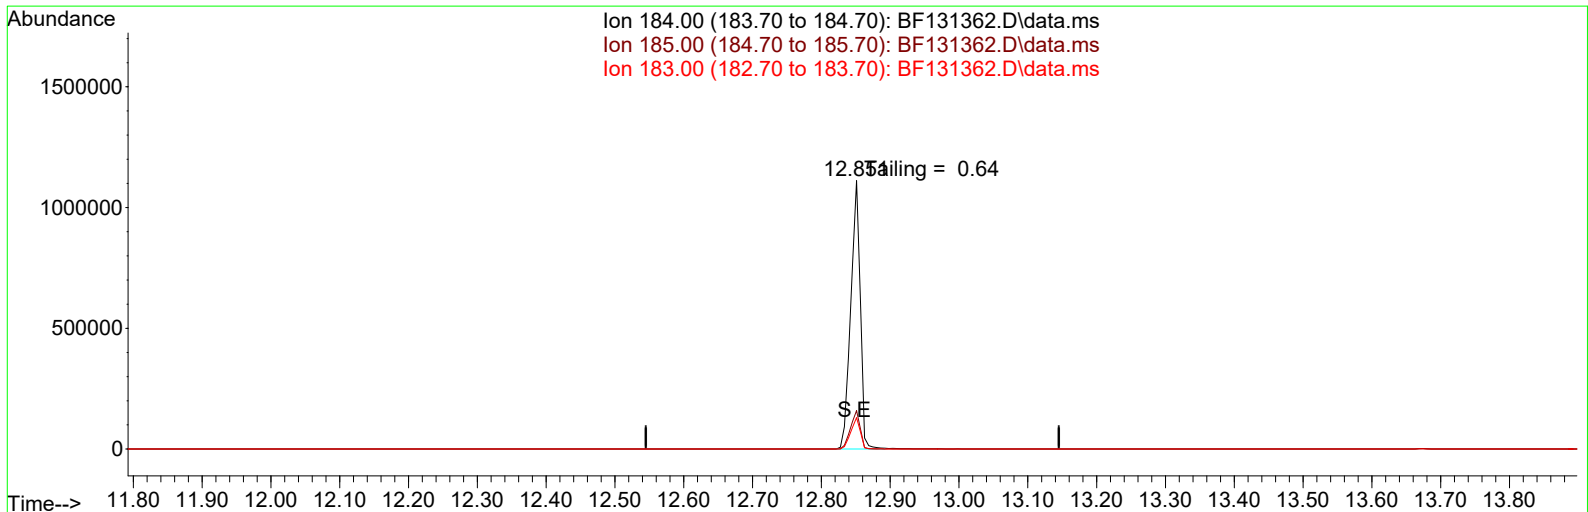

TIC: BF131362.D\data.ms

(77) Benzidine

12.845min (-12.845) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	17.30	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2022	BNA_F	<u>BF131362.D</u>
Compound Name	Response	Retention Time
DDT	432489	13.674
DDD	6528	13.404
DDE	115	13.033
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6643	439132	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP