

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122468.D
 Acq On : 24 Nov 2020 15:27
 Operator : JU/CG
 Sample : L4858-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-012

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.158	5	12	26	rVB	249178	450989	5.68%	0.455%
2	5.069	502	507	515	rVB	954312	1267111	15.95%	1.278%
3	5.487	572	578	581	rBV	3771865	3944758	49.65%	3.980%
4	5.869	639	643	650	rVB	155727	141338	1.78%	0.143%
5	6.493	744	749	754	rBV2	3843864	4544506	57.19%	4.585%
6	6.693	778	783	786	rBV4	91669	121920	1.53%	0.123%
7	6.851	807	810	818	rVB	1223421	1215794	15.30%	1.227%
8	7.104	848	853	856	rBV	234112	216937	2.73%	0.219%
9	7.257	872	879	888	rBV	393624	576798	7.26%	0.582%
10	7.416	896	906	909	rBV	2721970	2846680	35.83%	2.872%
11	7.457	910	913	916	rVB	166457	152749	1.92%	0.154%
12	7.792	966	970	978	rVB	448781	557106	7.01%	0.562%
13	7.904	984	989	991	rVV2	208964	305398	3.84%	0.308%
14	7.922	991	992	997	rVV2	211690	182206	2.29%	0.184%
15	7.963	997	999	1002	rVB	136292	109052	1.37%	0.110%
16	8.087	1016	1020	1024	rBV2	127989	157585	1.98%	0.159%
17	8.140	1024	1029	1032	rBV	1714606	1505323	18.95%	1.519%
18	8.292	1052	1055	1060	rBV	140323	122515	1.54%	0.124%
19	8.369	1065	1068	1071	rBV	138201	125521	1.58%	0.127%
20	8.487	1082	1088	1092	rBV3	377761	486935	6.13%	0.491%
21	8.534	1092	1096	1099	rVV2	82487	113123	1.42%	0.114%
22	8.569	1099	1102	1105	rVV2	159242	192978	2.43%	0.195%
23	8.598	1105	1107	1113	rVB	99112	114845	1.45%	0.116%
24	8.857	1148	1151	1156	rVB3	108746	132218	1.66%	0.133%
25	8.916	1157	1161	1164	rVV3	120358	139030	1.75%	0.140%
26	8.951	1164	1167	1171	rVB3	164286	169631	2.13%	0.171%
27	9.051	1180	1184	1186	rBV4	116692	135694	1.71%	0.137%
28	9.098	1186	1192	1198	rVV	1639057	1509490	19.00%	1.523%
29	9.163	1200	1203	1207	rVV	344578	331835	4.18%	0.335%
30	9.216	1207	1212	1216	rVB	5132926	5104188	64.24%	5.150%
31	9.298	1223	1226	1227	rBV	145356	124392	1.57%	0.126%
32	9.316	1227	1229	1231	rVV	262950	269912	3.40%	0.272%
33	9.334	1231	1232	1241	rVB	316647	298064	3.75%	0.301%
34	9.504	1258	1261	1264	rVB	643728	454358	5.72%	0.458%
35	9.581	1271	1274	1277	rBV2	209076	280267	3.53%	0.283%
36	9.610	1277	1279	1280	rBV	317415	246959	3.11%	0.249%
37	9.675	1287	1290	1294	rVB3	154928	191401	2.41%	0.193%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122468.D
 Acq On : 24 Nov 2020 15:27
 Operator : JU/CG
 Sample : L4858-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-012

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

38	9.745	1299	1302	1308	rBV2	196911	212804	2.68%	0.215%
39	9.798	1308	1311	1312	rBV	129421	140969	1.77%	0.142%
40	9.828	1314	1316	1321	rVV	230572	231822	2.92%	0.234%
41	9.898	1321	1328	1331	rVV	1864497	1961011	24.68%	1.979%
42	9.939	1331	1335	1341	rVV4	148528	268010	3.37%	0.270%
43	10.004	1343	1346	1350	rVB2	93512	110113	1.39%	0.111%
44	10.098	1358	1362	1367	rVB2	225137	241434	3.04%	0.244%
45	10.328	1399	1401	1404	rVB	246904	194058	2.44%	0.196%
46	10.551	1436	1439	1442	rVV2	198051	194118	2.44%	0.196%
47	10.598	1443	1447	1450	rVV3	78269	103881	1.31%	0.105%
48	10.686	1457	1462	1465	rBV	3633046	3305680	41.60%	3.335%
49	10.804	1479	1482	1487	rBV3	414227	659643	8.30%	0.666%
50	11.051	1521	1524	1531	rVB4	214279	262804	3.31%	0.265%
51	11.251	1555	1558	1560	rBV	322363	246697	3.10%	0.249%
52	11.280	1560	1563	1567	rVB	205958	205697	2.59%	0.208%
53	11.380	1577	1580	1583	rBV	1808298	1762314	22.18%	1.778%
54	11.404	1583	1584	1587	rVB	651530	392076	4.93%	0.396%
55	11.492	1596	1599	1602	rBV3	114924	131261	1.65%	0.132%
56	11.680	1628	1631	1633	rBV	360124	311312	3.92%	0.314%
57	11.728	1637	1639	1642	rVB	160068	136395	1.72%	0.138%
58	11.945	1664	1676	1680	rBV	4703082	7945743	100.00%	8.017%
59	12.075	1692	1698	1703	rBV3	1131995	1617940	20.36%	1.632%
60	12.204	1716	1720	1724	rVB	4012377	3857463	48.55%	3.892%
61	12.333	1737	1742	1745	rBV4	347226	436613	5.49%	0.441%
62	12.427	1755	1758	1759	rBV	372084	342502	4.31%	0.346%
63	12.457	1759	1763	1768	rVB	2783487	2988997	37.62%	3.016%
64	12.598	1784	1787	1789	rBV	808355	618696	7.79%	0.624%
65	12.651	1789	1796	1801	rVV2	2176105	4051383	50.99%	4.088%
66	12.722	1801	1808	1812	rVV2	3539182	4511381	56.78%	4.552%
67	12.827	1823	1826	1828	rVV	515496	385462	4.85%	0.389%
68	12.851	1828	1830	1831	rVV	280434	229445	2.89%	0.231%
69	12.892	1833	1837	1844	rVB2	843063	1578826	19.87%	1.593%
70	12.974	1847	1851	1854	rVB	4569092	4153085	52.27%	4.190%
71	13.110	1871	1874	1877	rVB	562157	444892	5.60%	0.449%
72	13.157	1880	1882	1886	rVB3	270413	255381	3.21%	0.258%
73	13.204	1887	1890	1894	rBV2	408548	377589	4.75%	0.381%
74	13.316	1906	1909	1912	rBV	694130	617439	7.77%	0.623%
75	13.457	1931	1933	1935	rBV2	747641	628829	7.91%	0.634%
76	13.545	1946	1948	1954	rVB	555146	530406	6.68%	0.535%
77	13.669	1966	1969	1973	rVB	1321526	1170552	14.73%	1.181%
78	13.710	1974	1976	1978	rVB2	239358	172023	2.16%	0.174%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122468.D
 Acq On : 24 Nov 2020 15:27
 Operator : JU/CG
 Sample : L4858-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-012

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

79	13.774	1981	1987	1990	rBV	1269656	2401701	30.23%	2.423%
80	13.857	1998	2001	2002	rBV2	457249	457897	5.76%	0.462%
81	13.874	2002	2004	2007	rVV	843701	951248	11.97%	0.960%
82	13.904	2007	2009	2013	rVB2	658594	583114	7.34%	0.588%
83	14.027	2026	2030	2032	rBV2	1385372	1381376	17.39%	1.394%
84	14.057	2032	2035	2039	rVB2	863036	899211	11.32%	0.907%
85	14.192	2055	2058	2063	rVB	638420	609841	7.68%	0.615%
86	14.321	2077	2080	2083	rVB	1543080	1307047	16.45%	1.319%
87	14.369	2085	2088	2091	rVV	1426166	1152372	14.50%	1.163%
88	14.421	2092	2097	2105	rVB	1536201	2499081	31.45%	2.521%
89	14.498	2107	2110	2116	rVB	594923	655235	8.25%	0.661%
90	14.568	2120	2122	2124	rBV	317769	231666	2.92%	0.234%
91	14.739	2148	2151	2157	rBV3	560763	750394	9.44%	0.757%
92	14.810	2160	2163	2166	rVB	434990	439035	5.53%	0.443%
93	14.998	2190	2195	2198	rBV	869703	1440082	18.12%	1.453%
94	15.033	2198	2201	2204	rVB	928135	964826	12.14%	0.973%
95	15.151	2218	2221	2229	rVB2	439233	631766	7.95%	0.637%
96	15.498	2276	2280	2283	rBV	932303	1098221	13.82%	1.108%
97	15.527	2283	2285	2291	rVB	320698	404621	5.09%	0.408%
98	15.651	2303	2306	2316	rVB2	470648	1122033	14.12%	1.132%
99	15.945	2351	2356	2364	rBV2	766630	1542985	19.42%	1.557%
100	16.333	2418	2422	2429	rBV	429495	765225	9.63%	0.772%




Sum of corrected areas: 99115329

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122468.D
Acq On : 24 Nov 2020 15:27
Operator : JU/CG
Sample : L4858-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-012

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

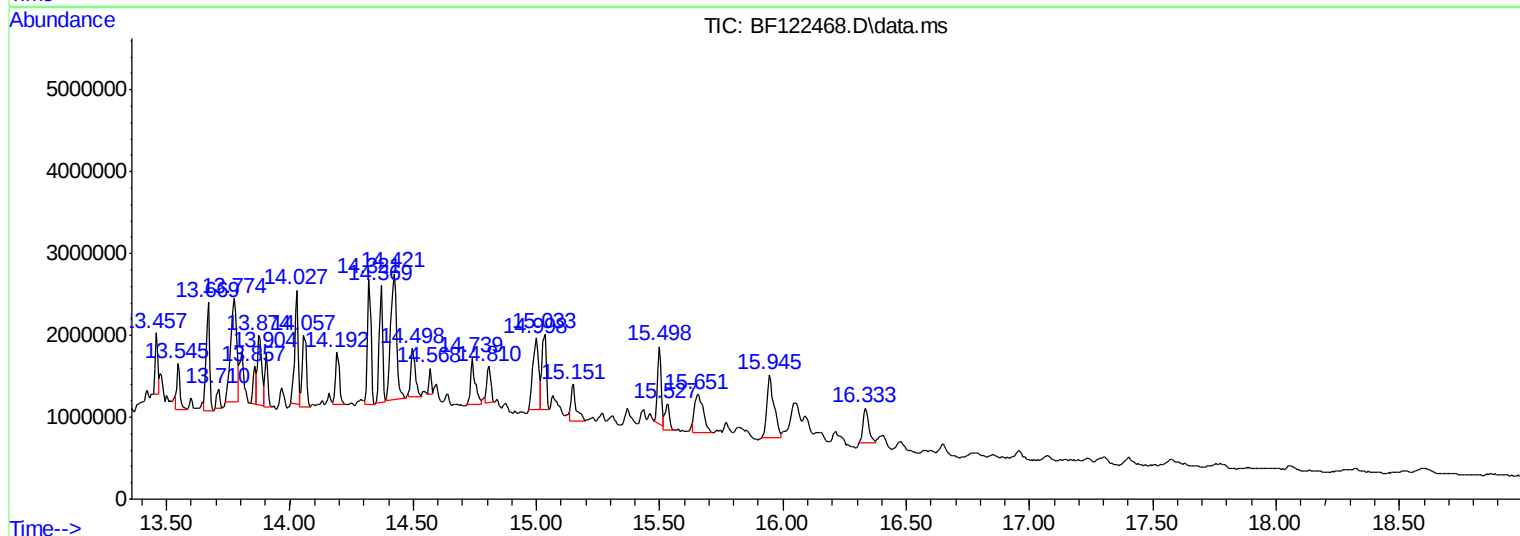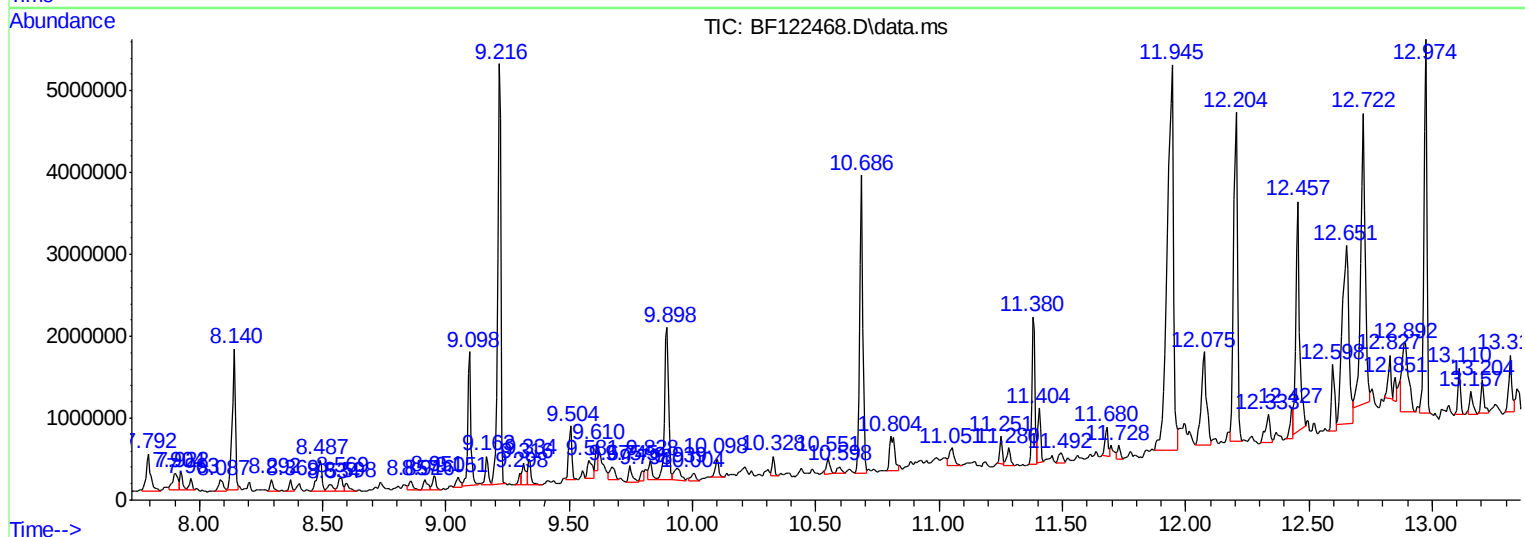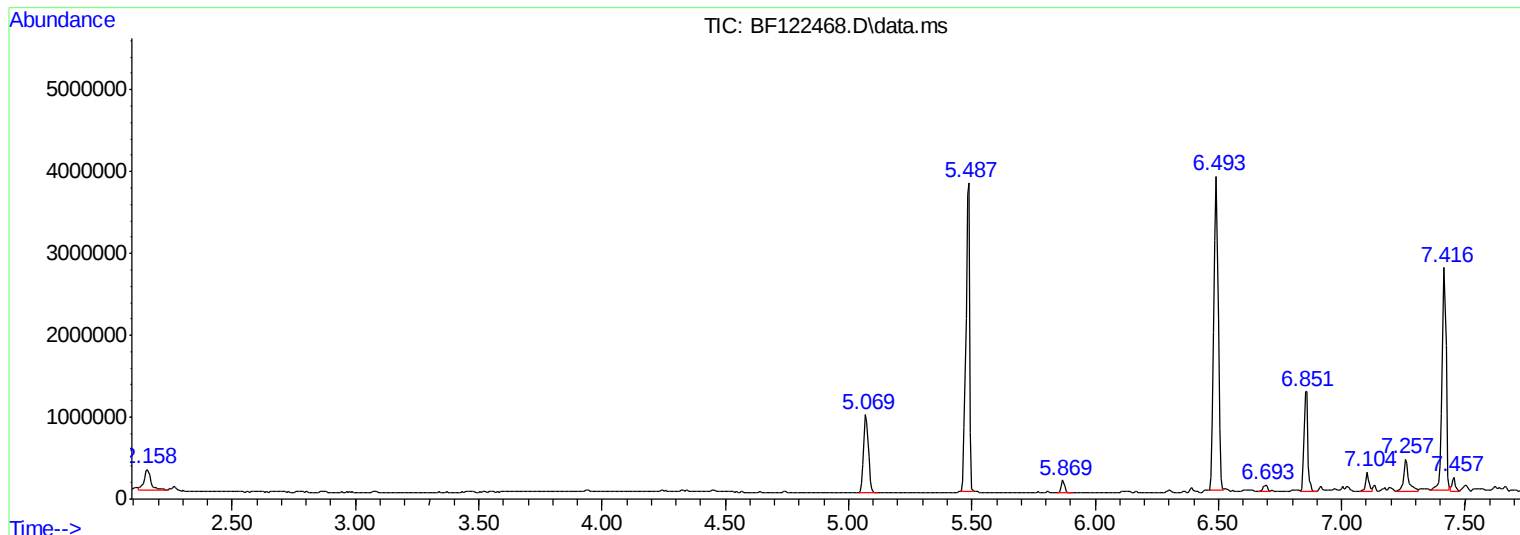

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122468.D
Acq On : 24 Nov 2020 15:27
Operator : JU/CG
Sample : L4858-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-012

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122468.D
Acq On : 24 Nov 2020 15:27
Operator : JU/CG
Sample : L4858-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-012

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc