

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122469.D
 Acq On : 24 Nov 2020 15:58
 Operator : JU/CG
 Sample : L4858-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-013

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	14	rVB	366110	477909	4.22%	0.245%
2	5.075	502	508	513	rBV	1050372	1354420	11.96%	0.694%
3	5.481	572	577	580	rVB	4067912	4340956	38.33%	2.226%
4	6.110	681	684	690	rVB4	377021	494570	4.37%	0.254%
5	6.392	728	732	734	rBV2	516955	647437	5.72%	0.332%
6	6.457	739	743	745	rBV2	383994	376102	3.32%	0.193%
7	6.492	745	749	754	rVV2	3890905	4709208	41.59%	2.414%
8	6.598	763	767	770	rBV2	322441	467282	4.13%	0.240%
9	6.681	779	781	786	rBV2	917546	1062227	9.38%	0.545%
10	6.857	807	811	812	rVV	1481212	1415549	12.50%	0.726%
11	6.875	812	814	818	rVV2	838196	799080	7.06%	0.410%
12	6.916	818	821	825	rVV2	798644	871847	7.70%	0.447%
13	7.004	833	836	840	rVV2	679155	783228	6.92%	0.402%
14	7.104	848	853	855	rVV5	541877	693594	6.13%	0.356%
15	7.134	855	858	861	rVB	936092	871563	7.70%	0.447%
16	7.175	861	865	867	rBV2	937008	935597	8.26%	0.480%
17	7.251	873	878	881	rVV2	993783	1065446	9.41%	0.546%
18	7.398	897	903	904	rVV3	1197264	1654498	14.61%	0.848%
19	7.422	904	907	911	rVV	2874280	3176984	28.06%	1.629%
20	7.457	911	913	917	rVB	824079	643988	5.69%	0.330%
21	7.504	917	921	925	rVB5	732662	965613	8.53%	0.495%
22	7.545	925	928	930	rBV2	364588	441641	3.90%	0.226%
23	7.569	930	932	935	rVV2	348819	376527	3.33%	0.193%
24	7.628	937	942	945	rVV3	508510	854788	7.55%	0.438%
25	7.657	945	947	952	rVB2	527010	720551	6.36%	0.369%
26	7.763	963	965	967	rVV2	398267	407673	3.60%	0.209%
27	7.786	967	969	973	rVV3	674894	930074	8.21%	0.477%
28	7.886	983	986	989	rVV3	1400329	1573334	13.89%	0.807%
29	7.957	994	998	1001	rVV5	233785	388325	3.43%	0.199%
30	8.139	1024	1029	1031	rVV	1831632	2104101	18.58%	1.079%
31	8.163	1031	1033	1036	rVV	1216625	972054	8.58%	0.498%
32	8.204	1036	1040	1042	rVV2	355263	400898	3.54%	0.206%
33	9.222	1207	1213	1216	rBV	4963169	4903375	43.30%	2.514%
34	9.486	1251	1258	1261	rBV2	252470	389826	3.44%	0.200%
35	9.610	1276	1279	1283	rVV2	472369	561411	4.96%	0.288%
36	9.757	1299	1304	1308	rBV	725686	642633	5.68%	0.329%
37	9.898	1321	1328	1331	rBV	2116282	1950923	17.23%	1.000%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122469.D
 Acq On : 24 Nov 2020 15:58
 Operator : JU/CG
 Sample : L4858-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-013

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

38	10.098	1359	1362	1365	rVB	523558	432895	3.82%	0.222%
39	10.445	1417	1421	1427	rVB2	650268	717593	6.34%	0.368%
40	10.545	1434	1438	1444	rVB3	382360	510865	4.51%	0.262%
41	10.686	1457	1462	1465	rVV	3836833	3504886	30.95%	1.797%
42	10.804	1479	1482	1490	rVB5	385421	684873	6.05%	0.351%
43	10.992	1509	1514	1516	rBV4	310440	403093	3.56%	0.207%
44	11.280	1560	1563	1568	rVB	568427	536176	4.73%	0.275%
45	11.386	1577	1581	1583	rBV	1783952	1853452	16.37%	0.950%
46	11.410	1583	1585	1588	rVV	3999803	3340703	29.50%	1.713%
47	11.457	1591	1593	1596	rVV	870546	705559	6.23%	0.362%
48	11.886	1663	1666	1668	rVV	1027302	994741	8.78%	0.510%
49	11.927	1668	1673	1677	rVV2	2278815	3680223	32.50%	1.887%
50	11.963	1677	1679	1682	rVV	394206	491282	4.34%	0.252%
51	11.998	1682	1685	1687	rVV2	1277687	1373765	12.13%	0.704%
52	12.021	1687	1689	1693	rVB	820393	678982	6.00%	0.348%
53	12.074	1694	1698	1704	rBV3	589468	994677	8.78%	0.510%
54	12.204	1711	1720	1725	rVB2	3589859	4268082	37.69%	2.188%
55	12.333	1736	1742	1745	rBV2	1097750	1286808	11.36%	0.660%
56	12.368	1745	1748	1750	rVV2	394789	455958	4.03%	0.234%
57	12.457	1753	1763	1766	rVV2	3572632	5198234	45.91%	2.665%
58	12.498	1768	1770	1772	rVV	513094	425513	3.76%	0.218%
59	12.521	1772	1774	1780	rVB6	538063	640046	5.65%	0.328%
60	12.604	1785	1788	1791	rBV	3550409	3215966	28.40%	1.649%
61	12.645	1791	1795	1798	rVV2	1682871	1786194	15.77%	0.916%
62	12.710	1801	1806	1811	rBV4	1943943	3064017	27.06%	1.571%
63	12.833	1824	1827	1833	rVB	3377596	3398841	30.02%	1.743%
64	12.910	1838	1840	1843	rVB2	466003	374008	3.30%	0.192%
65	12.945	1843	1846	1848	rBV3	386257	381112	3.37%	0.195%
66	12.974	1848	1851	1854	rVV	4343291	3879746	34.26%	1.989%
67	13.068	1861	1867	1871	rBV4	727842	1240198	10.95%	0.636%
68	13.115	1871	1875	1877	rVV	1198046	1291496	11.41%	0.662%
69	13.163	1880	1883	1887	rVB2	943327	961624	8.49%	0.493%
70	13.210	1888	1891	1892	rVV2	496971	484264	4.28%	0.248%
71	13.245	1895	1897	1899	rVV2	582977	627136	5.54%	0.322%
72	13.298	1903	1906	1911	rVV3	1020671	1181764	10.44%	0.606%
73	13.351	1912	1915	1918	rVV2	1950400	1752601	15.48%	0.899%
74	13.421	1925	1927	1930	rVV	686724	650810	5.75%	0.334%
75	13.463	1930	1934	1940	rVB3	2313175	2558566	22.59%	1.312%
76	13.551	1946	1949	1955	rBV4	444216	616200	5.44%	0.316%
77	13.604	1955	1958	1961	rVB	1727851	1562870	13.80%	0.801%
78	13.686	1966	1972	1974	rVV	7505541	9303354	82.16%	4.770%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
 Data File : BF122469.D
 Acq On : 24 Nov 2020 15:58
 Operator : JU/CG
 Sample : L4858-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PHC-340EM-013

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

79	13.721	1974	1978	1983	rVV	2589069	2264511	20.00%	1.161%
80	13.810	1990	1993	1996	rBV2	1164197	1165766	10.29%	0.598%
81	13.874	1998	2004	2008	rVV	5693954	11070412	97.76%	5.676%
82	13.915	2008	2011	2018	rVB2	5494637	6354970	56.12%	3.258%
83	13.980	2018	2022	2025	rBV	2590503	2440577	21.55%	1.251%
84	14.033	2026	2031	2034	rBV2	2219733	3233881	28.56%	1.658%
85	14.074	2034	2038	2041	rVB2	5483756	6265655	55.33%	3.212%
86	14.162	2051	2053	2055	rBV	928143	707107	6.24%	0.363%
87	14.345	2078	2084	2087	rVB	8633839	11323786	100.00%	5.806%
88	14.392	2087	2092	2095	rVB	8055313	8326858	73.53%	4.269%
89	14.580	2121	2124	2126	rBV	2466199	2218822	19.59%	1.138%
90	14.645	2132	2135	2138	rVB	1210098	1190991	10.52%	0.611%
91	14.757	2149	2154	2157	rVB	5542179	5881978	51.94%	3.016%
92	15.051	2198	2204	2207	rBV	5749966	7767785	68.60%	3.982%
93	15.086	2207	2210	2213	rVV2	658262	878549	7.76%	0.450%
94	15.309	2245	2248	2252	rVB	641251	699205	6.17%	0.358%
95	15.386	2258	2261	2267	rVB	749235	921297	8.14%	0.472%
96	15.451	2268	2272	2278	rVB	973029	1402443	12.38%	0.719%
97	15.515	2279	2283	2285	rBV	841654	1030699	9.10%	0.528%
98	15.951	2353	2357	2365	rVB3	514041	863915	7.63%	0.443%
99	16.339	2419	2423	2430	rBV	711074	1239334	10.94%	0.635%
100	16.974	2528	2531	2539	rVB2	452743	867184	7.66%	0.445%




Sum of corrected areas: 195050130

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122469.D
Acq On : 24 Nov 2020 15:58
Operator : JU/CG
Sample : L4858-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-013

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

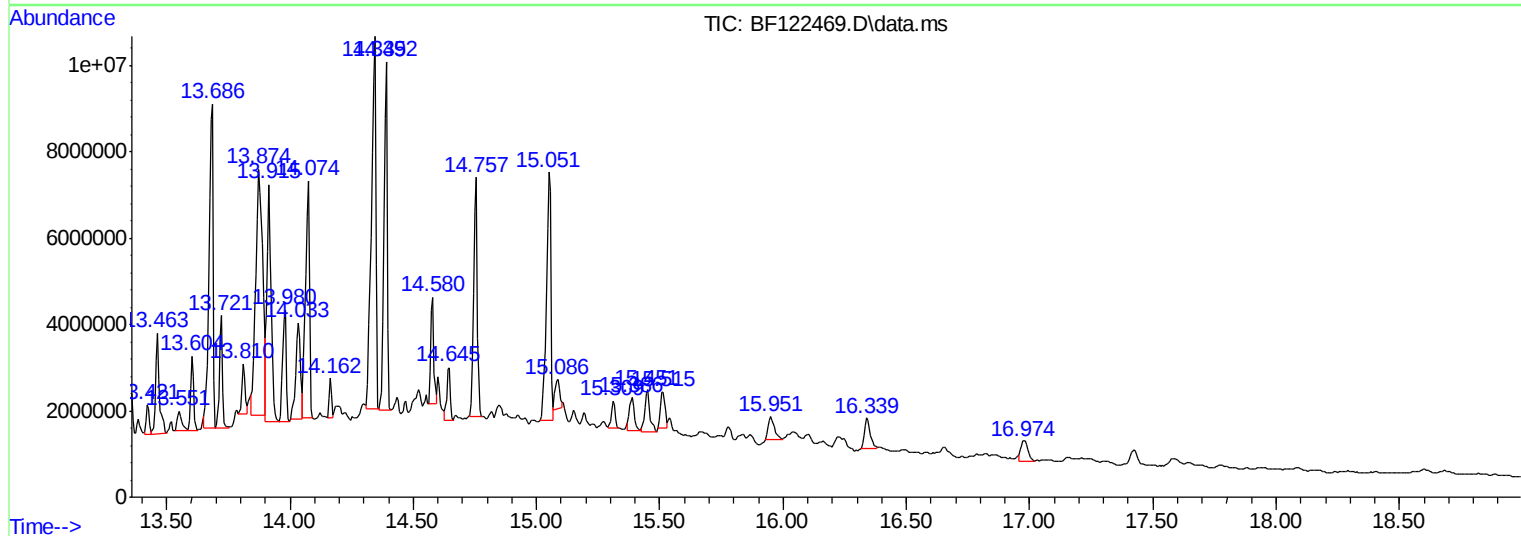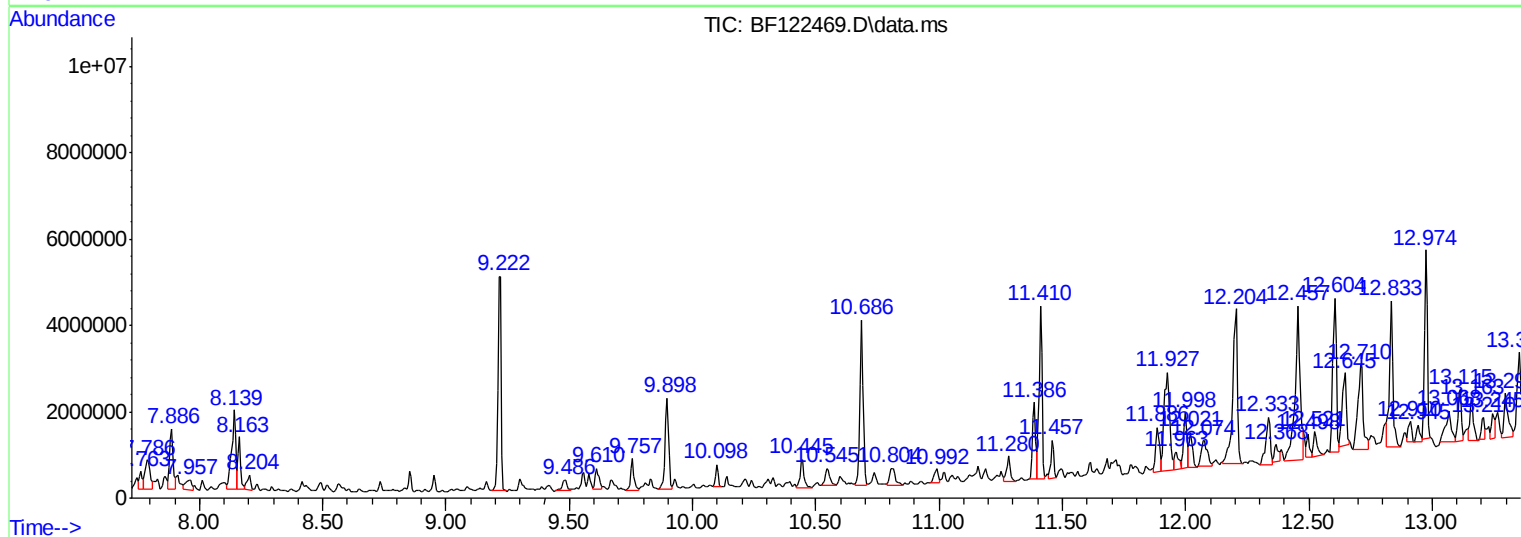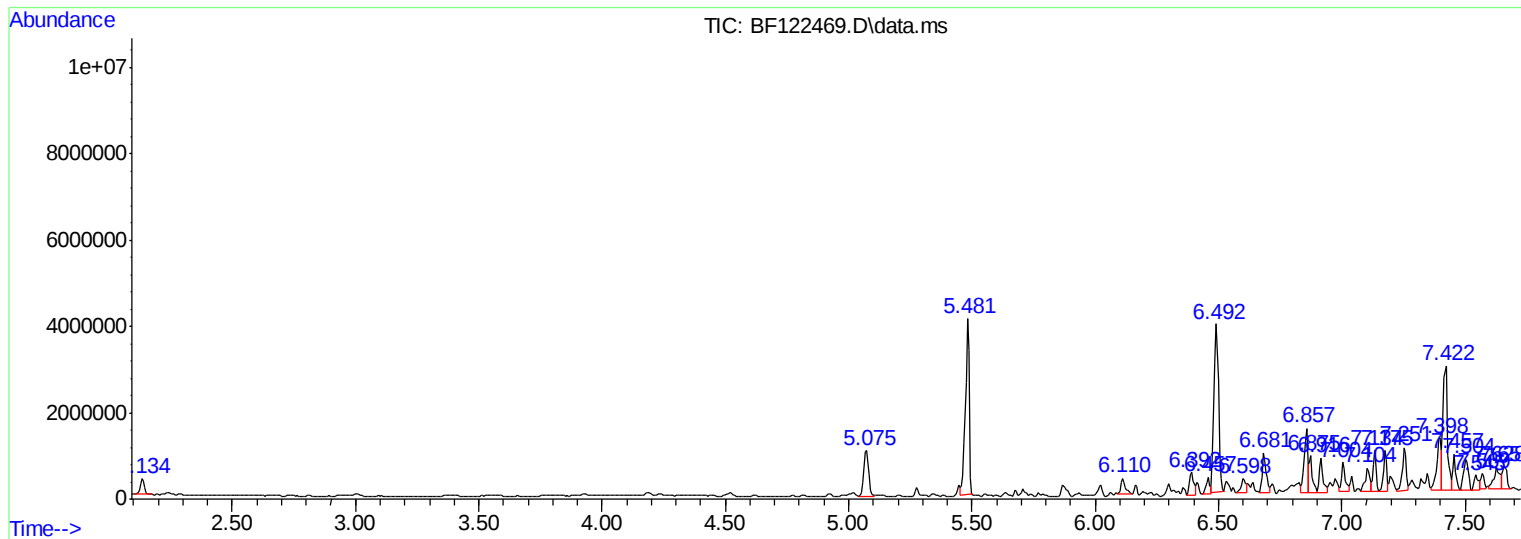

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122469.D
Acq On : 24 Nov 2020 15:58
Operator : JU/CG
Sample : L4858-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-013

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122469.D
Acq On : 24 Nov 2020 15:58
Operator : JU/CG
Sample : L4858-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PHC-340EM-013

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
