
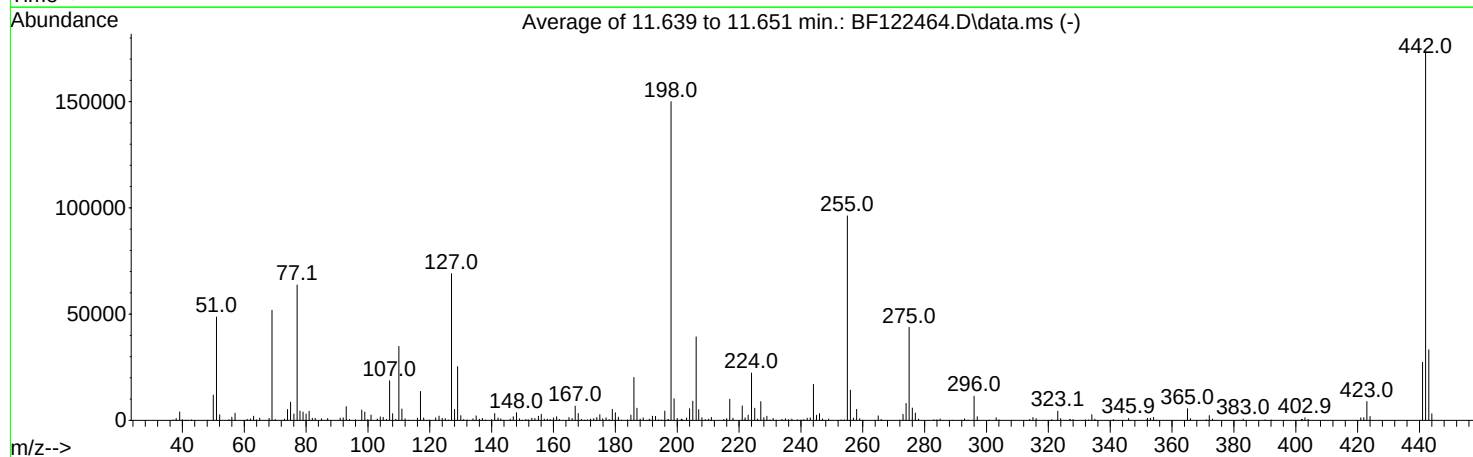


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112420\
Data File : BF122464.D
Acq On : 24 Nov 2020 13:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 24 14:38:56 2020

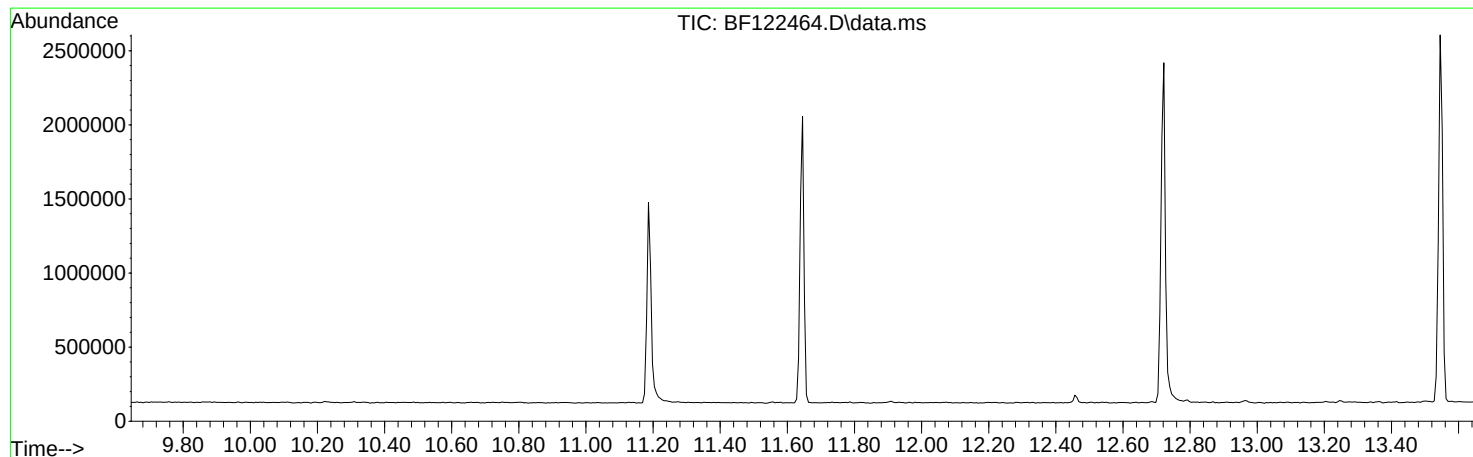

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	48647	PASS
68	69	0.00	2	1.8	916	PASS
69	198	0.00	100	34.6	51842	PASS
70	69	0.00	2	0.8	432	PASS
127	198	10	80	46.0	69048	PASS
197	198	0.00	2	0.3	468	PASS
198	198	100	100	100.0	149987	PASS
199	198	5	9	6.8	10144	PASS
275	198	10	60	29.2	43731	PASS
365	198	1	100	3.7	5516	PASS
441	198	0.01	100	18.2	27323	PASS
442	442	100	100	100.0	173117	PASS
443	442	15	24	19.2	33181	PASS