
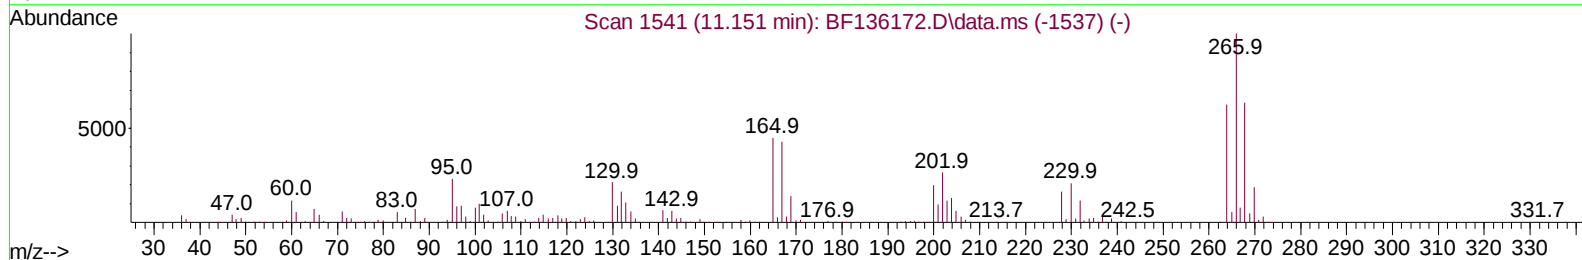
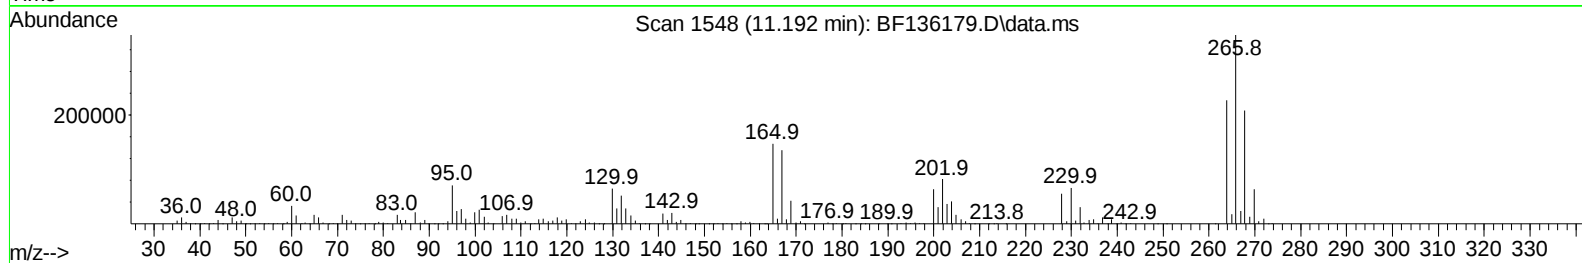


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136179.D
Acq On : 24 Nov 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 23:42:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:42:24 2023
Response via : Initial Calibration

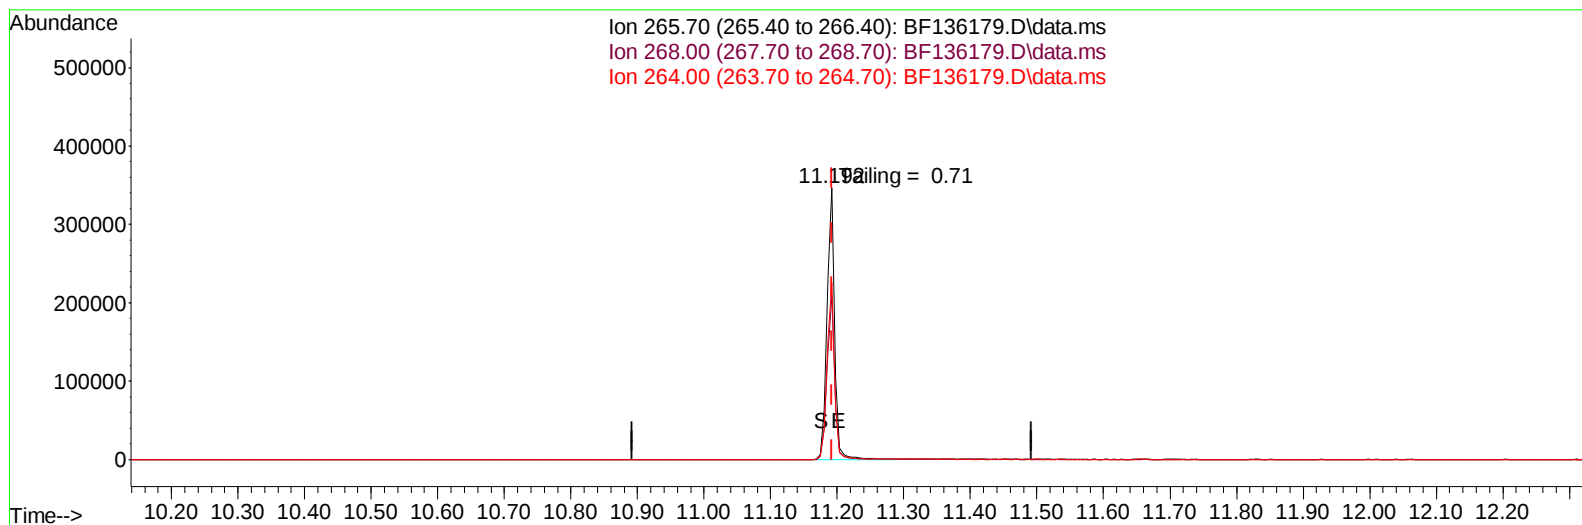

TIC: BF136179.D\data.ms




(70) Pentachlorophenol (C)

11.192min (0.000) 56831.47 ng

response 280373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	60.07
264.00	62.50	65.30
0.00	0.00	0.00

Quant Time: Nov 24 23:42:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:42:24 2023
Response via : Initial Calibration

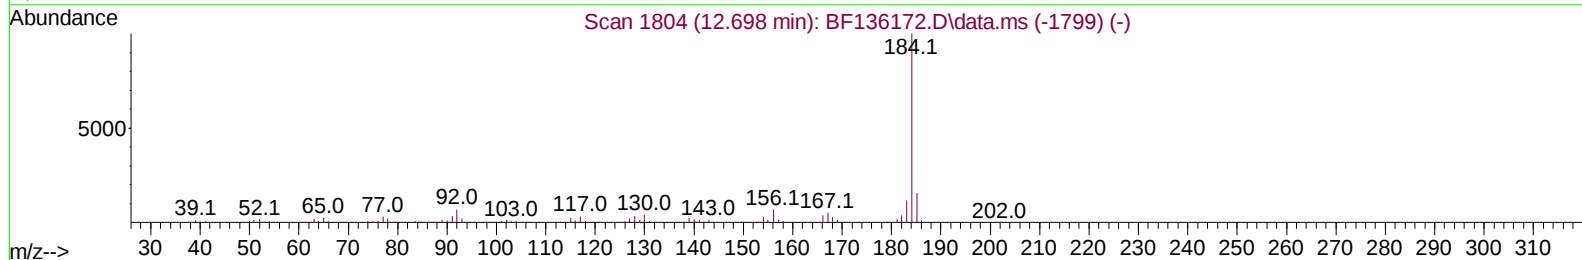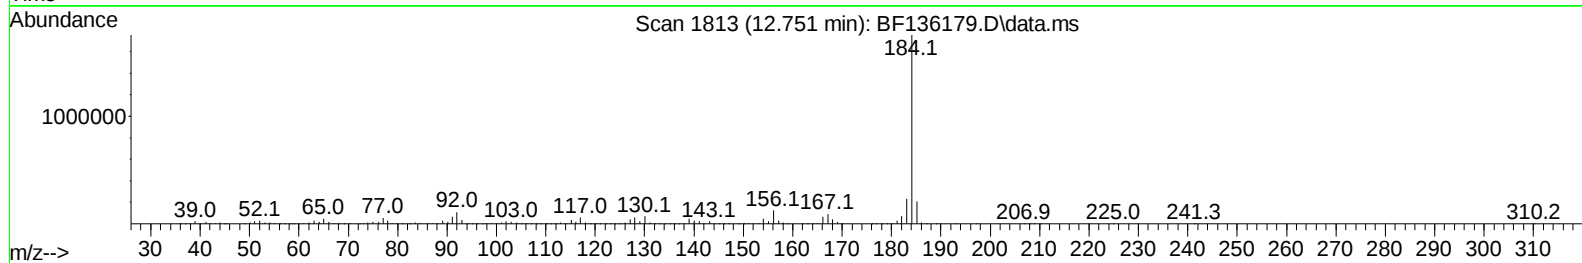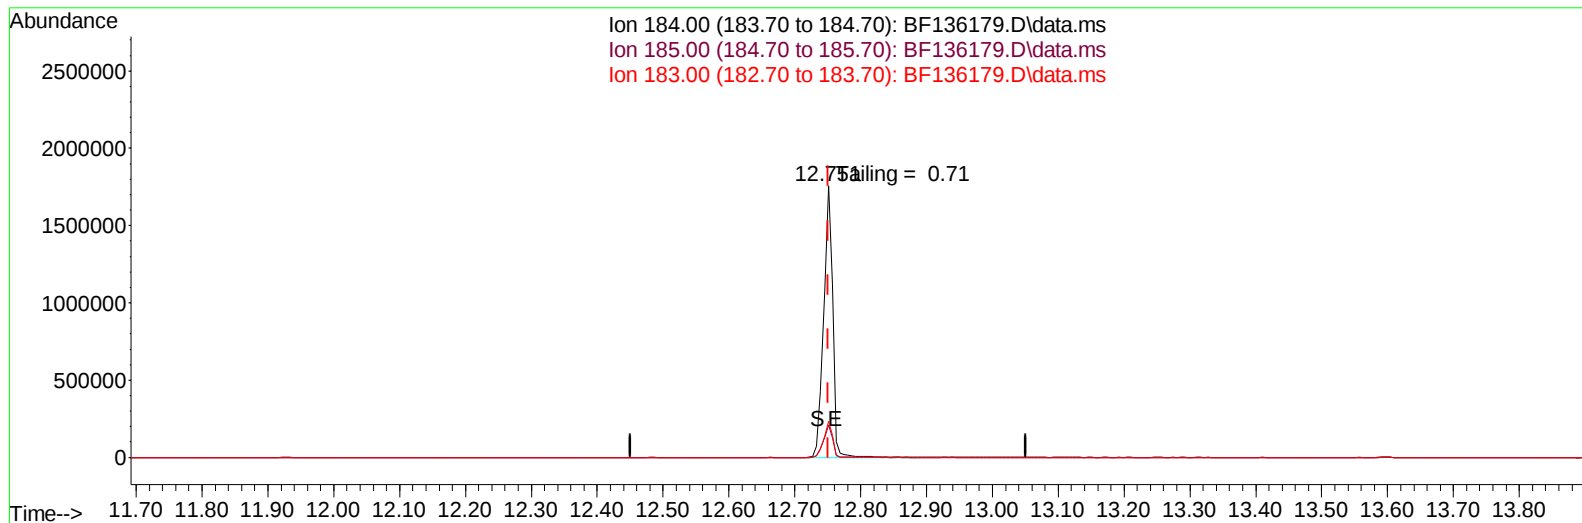

TIC: BF136179.D\data.ms

(77) Benzidine

12.751min (0.000) 133645.04 ng

response **1659250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	11.96#
183.00	11.50	13.31
0.00	0.00	0.00