
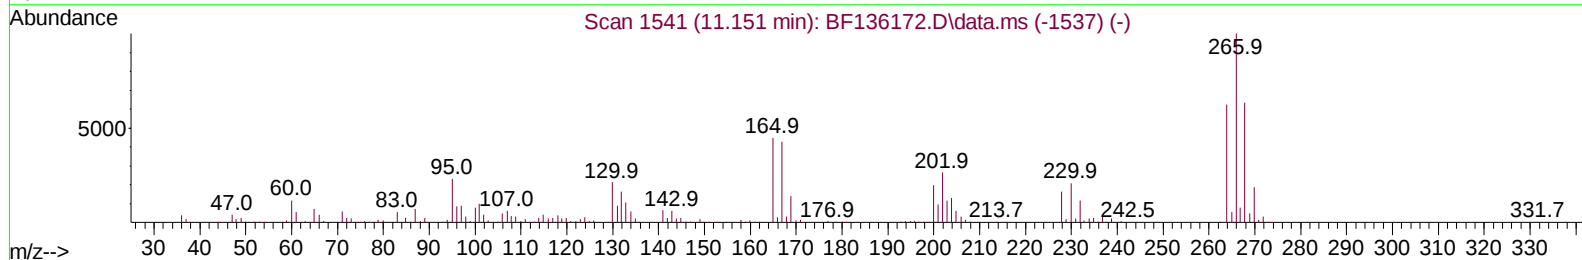
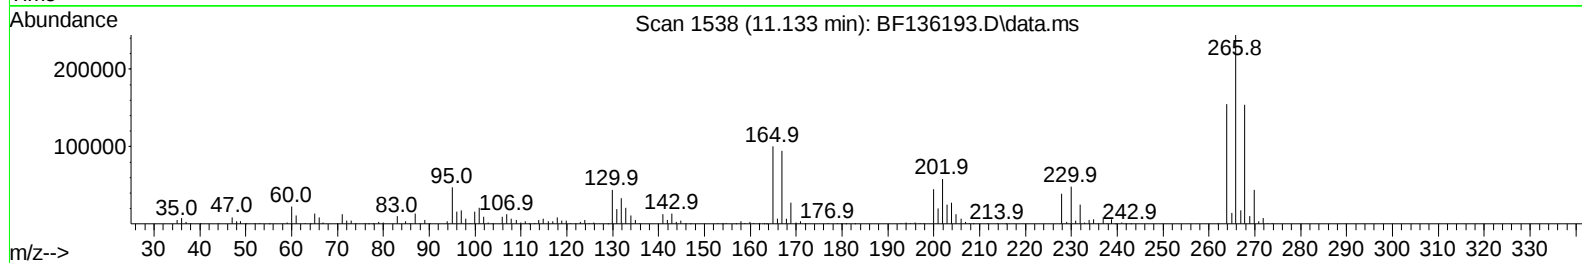


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136193.D
Acq On : 24 Nov 2023 23:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 24 23:44:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:44:28 2023
Response via : Initial Calibration

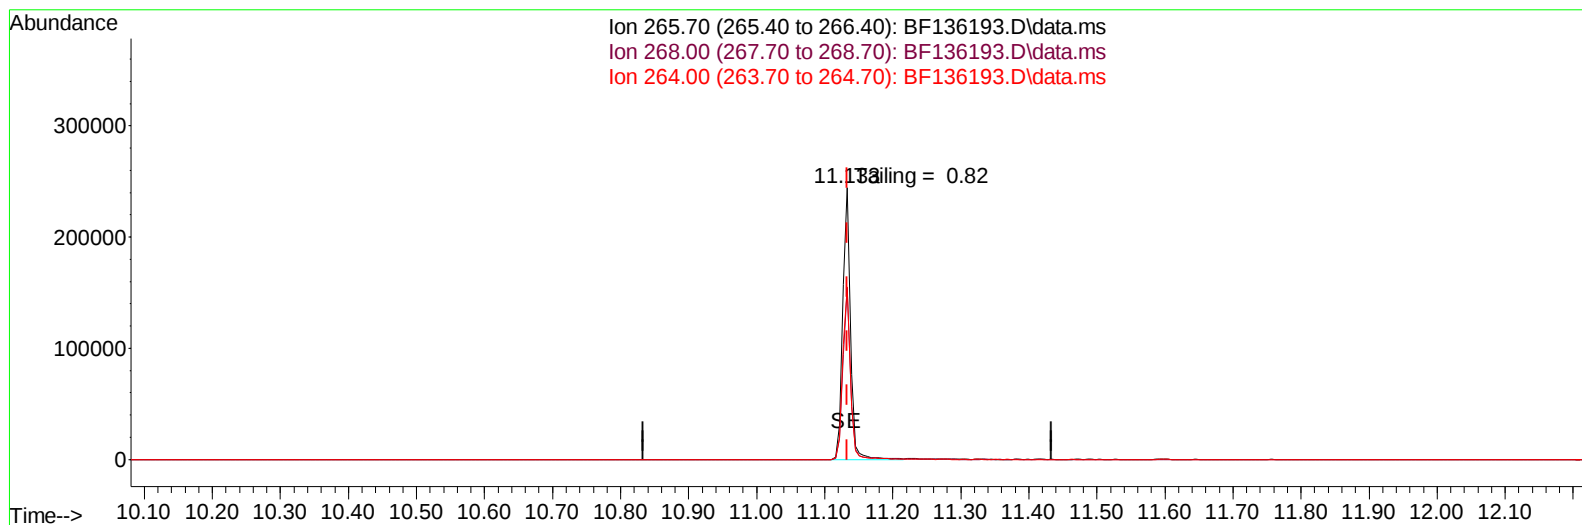

TIC: BF136193.D\data.ms

(70) Pentachlorophenol (C)




11.133min (0.000) 492949.43 ng

response 192337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.09
264.00	62.50	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136193.D
Acq On : 24 Nov 2023 23:00
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 24 23:44:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:44:28 2023
Response via : Initial Calibration

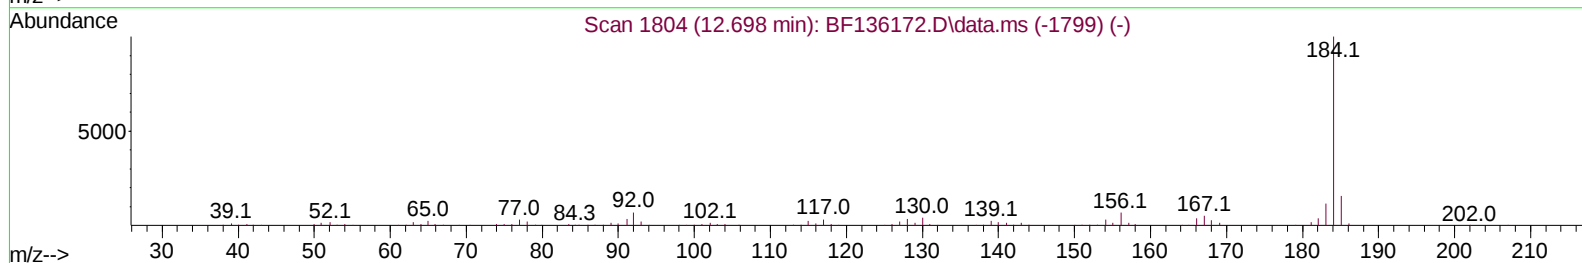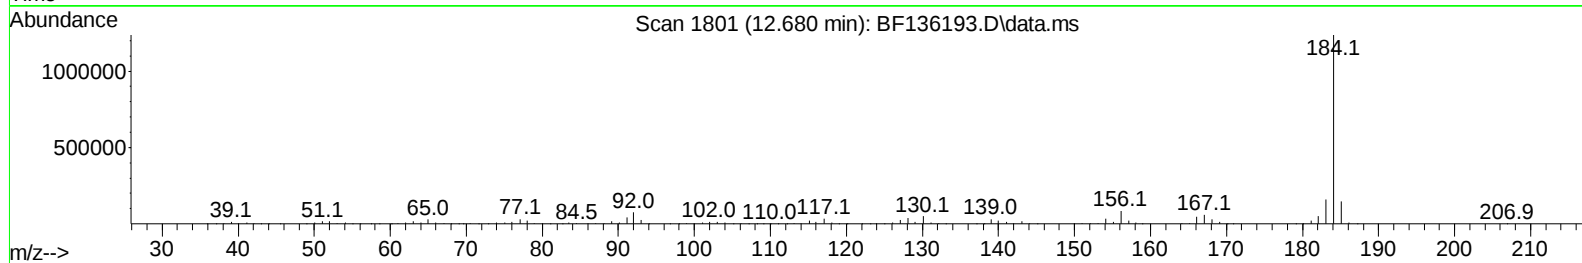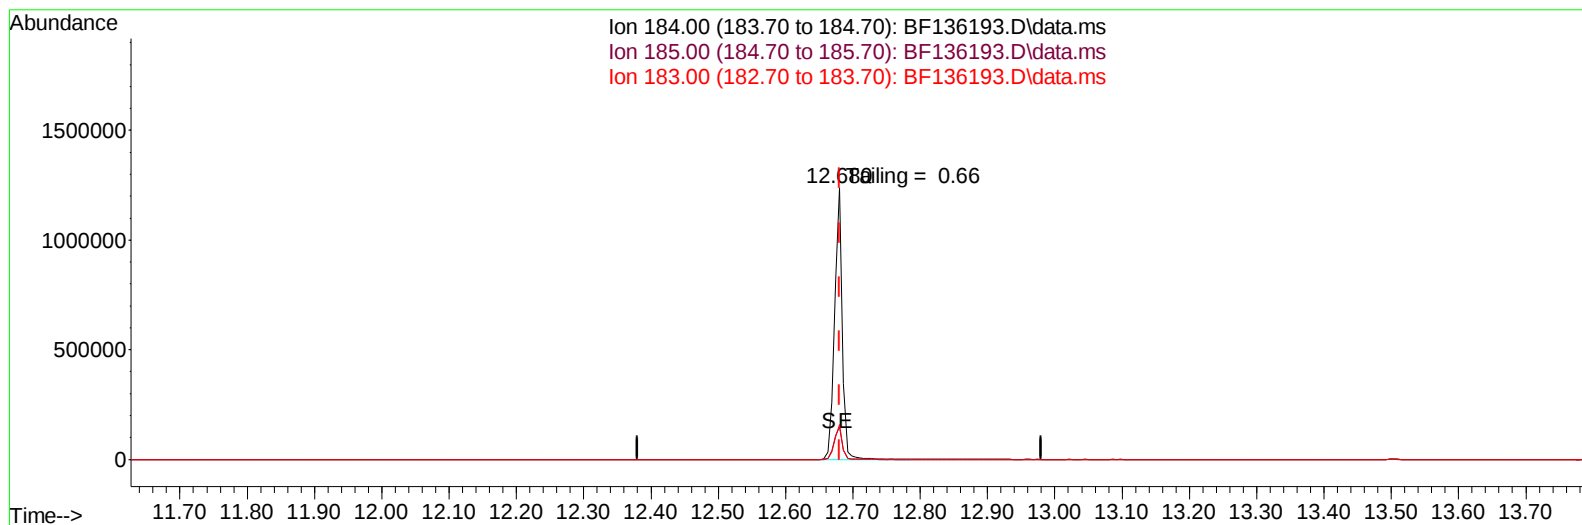

TIC: BF136193.D\data.ms

(77) Benzidine

12.680min (0.000) 0.00 ng

response 988426

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	11.84#
183.00	11.50	12.79
0.00	0.00	0.00