

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136181.D
 Acq On : 24 Nov 2023 16:01
 Operator : CG\JU
 Sample : PB157208BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157208BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	3	9	14	rVB	47030	66384	1.10%	0.202%
2	5.451	566	572	575	rBV	4447604	4525615	75.27%	13.737%
3	6.445	735	741	743	rBV	4178706	4423991	73.58%	13.429%
4	6.804	799	802	806	rBV	977238	803101	13.36%	2.438%
5	7.369	892	898	901	rBV	2989299	2778574	46.21%	8.434%
6	8.086	1015	1020	1023	rBV	1159607	1091787	18.16%	3.314%
7	9.163	1198	1203	1206	rBV	6058325	5935704	98.72%	18.018%
8	9.839	1313	1318	1322	rBV	1532616	1265473	21.05%	3.841%
9	10.633	1448	1453	1456	rBV	3518591	3152905	52.44%	9.571%
10	11.333	1568	1572	1575	rBV	1710525	1302737	21.67%	3.954%
11	12.933	1839	1844	1847	rBV	6403151	6012871	100.00%	18.252%
12	13.980	2018	2022	2026	rBV	900611	863263	14.36%	2.620%
13	15.468	2269	2275	2282	rBV	595717	721510	12.00%	2.190%




Sum of corrected areas: 32943915

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136181.D
Acq On : 24 Nov 2023 16:01
Operator : CG\JU
Sample : PB157208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

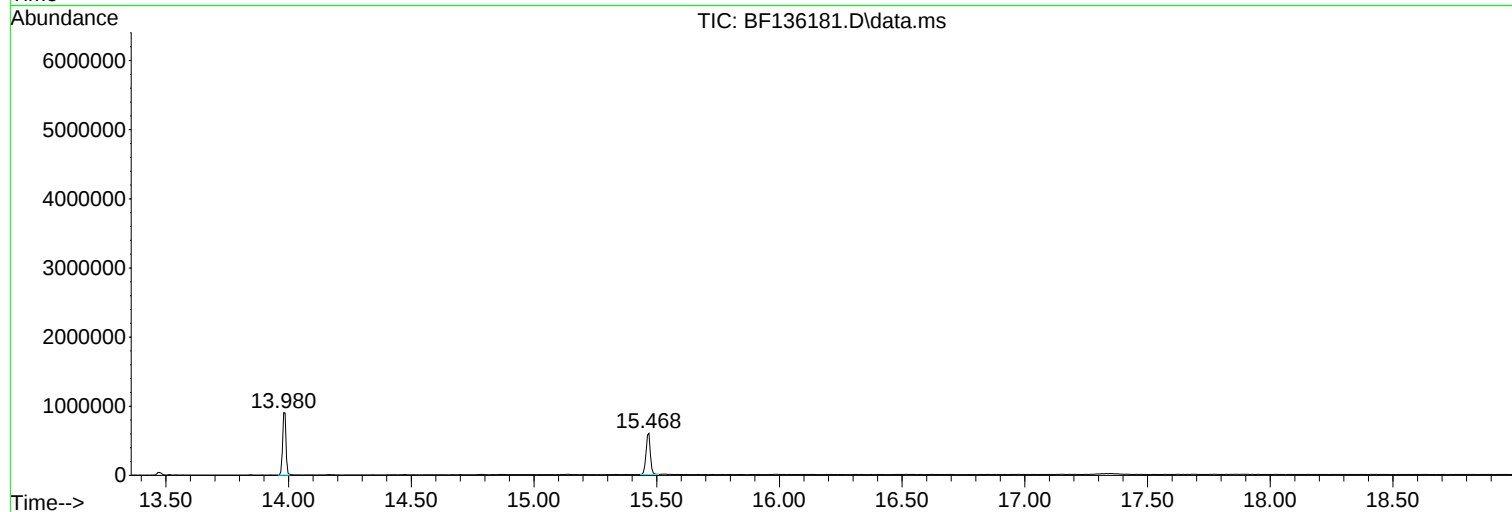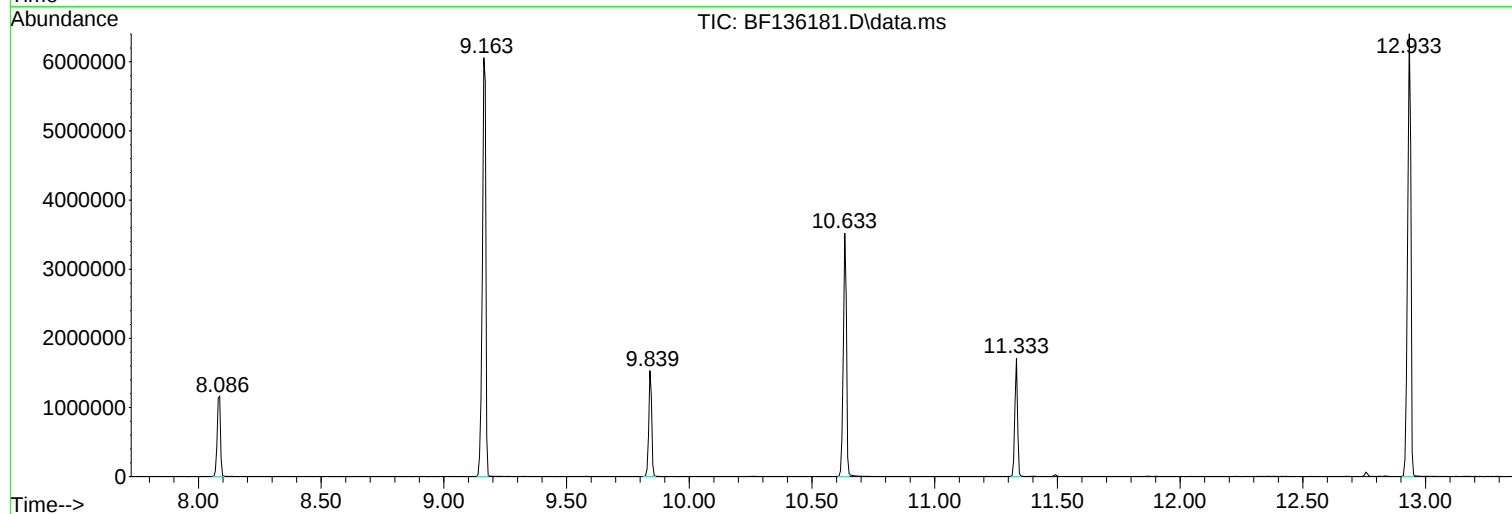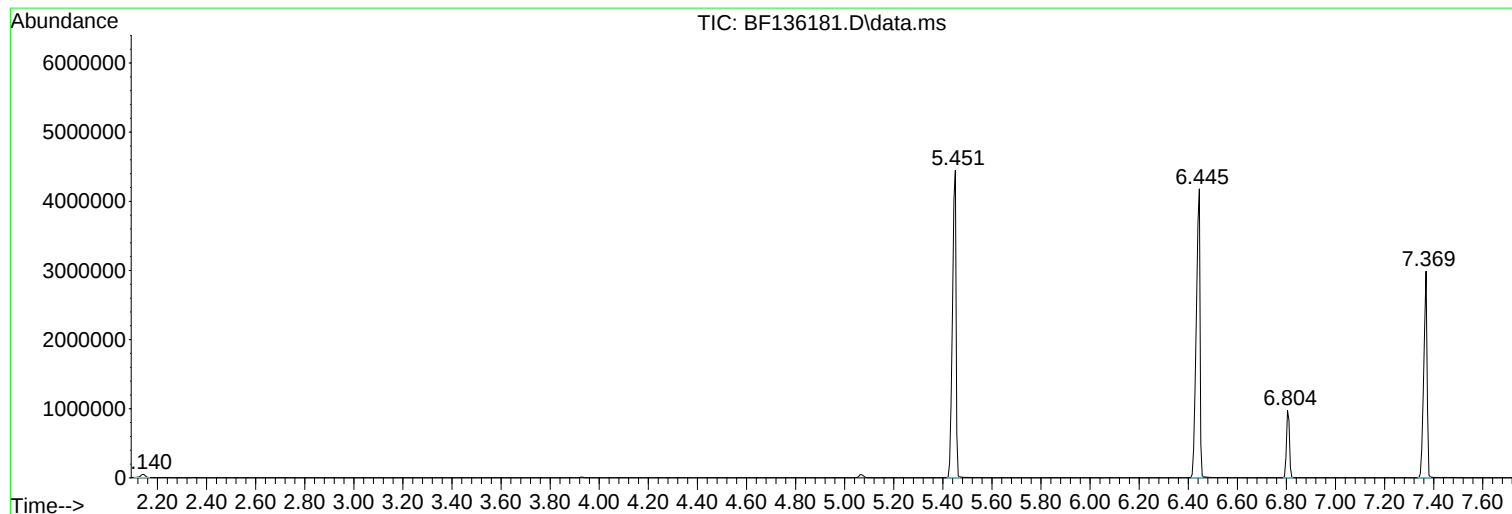

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136181.D
Acq On : 24 Nov 2023 16:01
Operator : CG\JU
Sample : PB157208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136181.D
Acq On : 24 Nov 2023 16:01
Operator : CG\JU
Sample : PB157208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------